



Space charge effects in high pressure mass spectrometry sources
by Mark Busman

A thesis submitted in partial fulfillment of the requirements for the degree of Doctor of Philosophy in Chemistry

Montana State University

© Copyright by Mark Busman (1991)

Abstract:

Ion transport in unipolar mass spectrometry ion sources like corona API and electrospray has been studied theoretically. Unlike previous work in this area, the study has been done with the consideration of space charge effects. Analytic solutions of the space charge problem have been obtained for simple ion geometries, including the cases of infinite parallel planes, concentric cylinders of infinite length, and concentric spheres. These analytic solutions allow, for their respective geometries, the calculation of electric field, potential, ion density distributions, and ion residence times. It is shown that for typical operating conditions, the minimum potential required to overcome the space charge effect in corona API, or electrospray ion sources, constitutes a dominant or significant fraction of the total applied voltage. Further, the electric field, in the region of the ion sampling orifice and the ion residence time in the ion source are determined mainly by the space charge. Extending the approach to more general geometries, absolute sensitivities of corona API ion sources were calculated using a geometry independent treatment of space charge. Also, general geometries were modelled by a simulation calculation. The calculation was based on a computer program written to model ion flow in various ion sources having different geometries. Finally, the space charge influenced ion drift in a drift tube-type apparatus was modelled, as a function of time.

SPACE CHARGE EFFECTS IN HIGH PRESSURE
MASS SPECTROMETRY SOURCES

by

Mark Busman

A thesis submitted in partial fulfillment
of the requirements for the degree

of

Doctor of Philosophy

in

Chemistry

MONTANA STATE UNIVERSITY
Bozeman, Montana

July 1991

D378
B9655

APPROVAL

of a thesis submitted by

Mark Busman

This thesis has been read by each member of the thesis committee and has been found to be satisfactory regarding content, English usage, format, citations, bibliographic style, and consistency, and is ready for submission to the College of Graduate Studies.

June 24, 1991
Date

Jan Sumner
Chairperson, Graduate Committee

Approved for the Major Department

June 24, 1991
Date

Edwin H. Abbott
Head, Major Department

Approved for the College of Graduate Studies

August 12, 1991
Date

Henry L. Parsons
Graduate Dean

STATEMENT OF PERMISSION TO USE

In presenting this thesis in partial fulfillment of the requirements for a doctoral degree at Montana State University, I agree that the Library shall make it available to borrowers under rules of the Library. I further agree that copying of this thesis is allowable only for scholarly purposes, consistent with "fair use" as prescribed in the U.S Copyright Law. Requests for extensive copying or reproduction of this thesis should be referred to University Microfilms International, 300 North Zeeb Road, Ann Arbor, Michigan 48106, to whom I have granted "the exclusive right to reproduce and distribute copies of the dissertation in and from microfilm and the right to reproduce and distribute by abstract in any format."

Signature Mark Busma

Date June 24, 1991

TABLE OF CONTENTS

	Page
INTRODUCTION	1
Ion Transport	2
Convective Transport	2
Diffusive Transport	3
Electrostatic Transport	3
MATHEMATICAL TREATMENT OF ION TRANSPORT	4
Drift Equation	4
Laplacian Field	5
Space Charge Field	5
Historical Background	6
Mathematical Background	8
Analytic Solutions	10
Planar	10
Cylindrical	12
Spherical	18
APPLICATIONS OF THE ANALYTIC SOLUTIONS	24
Corona API in the Spherical Geometry	27
Electrospray in the Spherical Model	33
GENERAL GEOMETRIES	38
Unipolar Charge Drift Formula	38
Calculation of Absolute Sensitivities	45
Numeric Solutions	51
Simulation Method	55
Simulation in General Geometries	56
Point to Plane Geometry	62
Electrospray Geometry	62
API Geometry	67
TIME DEPENDENT CASE	72
Simulation With One Type of Ion	74
Simulation With Two Types of Ions	76
SUMMARY	80
REFERENCES CITED	82

TABLE OF CONTENTS-Continued

	Page
APPENDICES	86
APPENDIX A: ANALYTIC SOLUTIONS	87
Planar geometry	88
Cylindrical Geometry	90
Spherical geometry	92
APPENDIX B: DERIVATIONS FOR LIMITING CONDITIONS .	95
Ion residence time, t_{res}	96
Sampling ion density, ρ_{smp}	97
Applied potential, V_0	98
APPENDIX C: COMPUTER PROGRAMS	99

LIST OF FIGURES

Figure	Page
1. Planar Geometry.	11
2. Non-SCD Residence Time and Space Charge.	13
3. SCD Residence Time and Space Charge.	14
4. Non-SCD Potential and Fields.	15
5. SCD Potential and Fields.	16
6. Cylindrical Geometry.	17
7. SCD and Non-SCD Fields.	19
8. SCD and Non-SCD Space Charge Densities.	20
9. Spherical Geometry.	21
10. SCD Conditions in the Spherical Geometry.	23
11. Schematic of the Corona-API.	28
12. Conditions in the Corona-API.	30
13. Residence Time, Potential and Ion Density	34
14. Schematic of the Electrospray.	35
15. Ion Density vs. Drift Time.	40
16. Field strength map for the nonfocussed case.	42
17. Field strength map for the focussed case.	42
18. Ion density contour for the unfocussed case.	43
19. Ion density contour for the focussed case.	43
20. Current densities for the Case 1 and Case 2.	44
21. Ion densities for the Case 1 and Case 2.	44
22. Kinetically Influenced API Currents.	50
23. Calculated API Currents.	52
24. Experimental API Currents.	53
25. Point to Plane Geometry.	57
26. "Needle in Can" Geometry.	58
27. Parabolic Grid.	59
28. Point to Plane Plate Current Distribution.	63
29. Electrospray Plate Current Distribution.	64
30. Spray Pattern from a Taylor Cone.	65
31. Spray Pattern from the "Umbrella" Mode.	66
32. Calculated Electrospray Current Distribution.	68
33. Field and Space Charge Density Contour.	69
34. Calculated Corona-API Current Distribution.	70
35. Corona-API Field, Space Charge Contour.	71
36. Ion Tube in the Fenn Electrospray Source.	73
37. Drift Tube Schematic.	75
38. One Component Ion Drift Current vs. Time.	77
39. Two Component Ion Drift Current vs. Time.	78
40. SPACE.BAS.	100
41. SPREAD.BAS.	119

LIST OF FIGURES-Continued

Figure	Page
42. TUBE.M.	124
43. TUB2.M.	126
44. VELOCITY.M.	128
45. DISPLACEMENT.M.	129

ABSTRACT

Ion transport in unipolar mass spectrometry ion sources, like corona API and electrospray has been studied theoretically. Unlike previous work in this area, the study has been done with the consideration of space charge effects. Analytic solutions of the space charge problem have been obtained for simple ion geometries, including the cases of infinite parallel planes, concentric cylinders of infinite length, and concentric spheres. These analytic solutions allow, for their respective geometries, the calculation of electric field, potential, ion density distributions, and ion residence times. It is shown that for typical operating conditions, the minimum potential required to overcome the space charge effect in corona API, or electrospray ion sources, constitutes a dominant or significant fraction of the total applied voltage. Further, the electric field, in the region of the ion sampling orifice and the ion residence time in the ion source are determined mainly by the space charge. Extending the approach to more general geometries, absolute sensitivities of corona API ion sources were calculated using a geometry independent treatment of space charge. Also, general geometries were modelled by a simulation calculation. The calculation was based on a computer program written to model ion flow in various ion sources having different geometries. Finally, the space charge influenced ion drift in a drift tube-type apparatus was modelled, as a function of time.

INTRODUCTION

In the last half century, mass spectrometry has gradually evolved from being an interesting tool for the mass measurement of relatively small ions, into a vital area of analytical chemistry. This evolution has followed the development of creative techniques for the introduction of molecules into an ion source for mass analysis, and achieving their ionization.

The ion sources used in mass spectrometry can be classified according to source pressures. Sources operated at pressures 1 torr and below can be considered to be low pressure ion sources. Low pressure sources include sources for many of the more commonly used mass spectrometry techniques: electron impact ionization (EI),^{1,2} chemical ionization (CI),³ and fast atom bombardment (FAB).⁴ High pressure ion sources can be thought to be those that operate in the pressure range between 1 torr and atmospheric pressure, and perhaps beyond. High pressure sources include the sources used for atmospheric pressure ionization (API),⁵ thermospray ionization (TSP),⁶ and electrospray ionization (ES).^{7,8} The ion sources in both of these categories have been studied to establish appropriate parameters for their operation. Much has been written with

respect to the mechanisms pertinent to the operation of these sources.

In mass spectroscopy, the understanding of the production of ions in the ion source is an important aspect of understanding the technique. Further, understanding the processes behind introducing the ions into the mass resolution part of the instrument is vital for insight into the identities and quantities of ions available for detection. The goal of this work is to evaluate certain aspects of ion transport in high pressure mass spectrometry sources with regard to the performance of these sources.

Ion Transport

In the ion source of the mass spectrometer ions are produced from existing molecules. These ions are then driven toward an aperture separating the high-pressure ion source from the low-pressure mass analyzer section of the mass spectrometer, where they can travel towards the detector. The processes causing the ions to leave the ion source can be of the following types of transport: convective, diffusive, and electrostatic.

Convective Transport

The ion source is often at much higher pressure than the mass analyzer region. The ions will be carried along with the gas stream down the pressure gradient. The study of

how ions can flow along with a moving gas is an important area in fluid dynamics.⁹

Diffusive Transport

In many ion sources, ions are not formed throughout the source, but, instead, are formed in a small volume in the ion source. Here, the concentration of ions may be very high. The ions tend to diffuse out of the areas of high concentration into areas of lower concentration. The mathematical treatment of the diffusion of ions in gases is well developed.^{10,11}

Electrostatic Transport

Ions, as charged species, will drift in existing fields. An ion will drift in the direction of existing electrical fields. The drift velocity depends on the field's intensity. Again, the mathematical treatment of ionic drift has already been developed.^{9,11} Ion drift will now be discussed in more detail.

MATHEMATICAL TREATMENT OF ION TRANSPORT

The application of electrostatics to charged particle flow and, in particular, ion flow has been important to physics for many years. The analysis ion flow has been based on Coulomb's and Maxwell's equations.¹² It is these equations that make the analysis of ion drift in the mass spectrometer ion source possible.

Drift Equation

Using appropriate laws of electrostatics, one can predict the magnitude and direction of the forces acting upon ions at specific locations in the source. Moreover, assuming certain characteristics of both the ions, and the neutral gas inside the source, one can predict a velocity for an ion under the influence of a given field. This velocity, the drift velocity, v , can be given as a function of electric field strength, E , by the drift equation,

$$v = \kappa \cdot E, \quad (1)$$

where κ is the ion mobility, a constant, dependent on both the characteristics of the ion and its surrounding gas, and generally assumed to be independent of field strength.^{10,13}

The drift equation is essentially an empirical equation that summarizes a large amount of experimental data. It has been shown to be applicable at high pressures (above 1 torr). The mobility, κ , is the empirical constant in the equation. The mobility constant's magnitude is dependent on the charged particle's response to an electric field and to the collisions with the neutral bath gas that the particle will experience. Compilations of mobility data have been published, most notably by McDaniel.¹³

Laplacian Field

An ion source often has several electrically insulated components that have different applied potentials. From the geometry of the ion source, it is possible, in theory, to map out the electric fields in the source, that result from the application of the potentials to the various source components.¹⁴ Generally, it is assumed that the field strength at any point in the source is dependent on only the external applied field. The field strength at any point is determined by the source geometry and the respective applied voltages on various source components. This external field is commonly called the Laplacian field.¹¹

Space Charge Field

As ion densities in the source increase, the coulombic forces between the ions will increasingly modify the

Laplacian electrical fields experienced by ions. In the source the conduction of current will be unipolar. By saying that the current is unipolar, it is meant that particles of only one polarity exist in the source, and that the ion flow can be considered accordingly. The ions in the ion source, traveling at finite velocities, experience a mutual coulombic repulsion during the time that they transit the gap between electrodes, thus forming their own electric field. The Laplacian field is combined with the field caused by the moving charge, the space charge field. This combination is the actual field experienced by the ions. In the extreme, the space charge field, from the unipolar current, can be so large that it completely dominates any applied field.

Historical Background

The modification of Laplacian fields by space charge was noticed many years ago by workers studying electrical currents between charged plates. As they attempted to increase the current between these charged plates by changing the conditions between the plates, they found that it was not possible to increase the current beyond a certain limiting current. This was explained by the modification of the fields between the plates, by the current flow.^{15,16,12}

The mathematical picture of space charge was initially developed by Child, in 1908, to model the evaporation of

calcium ions from a heated plate.¹⁵ Unaware of Child's work, Langmuir, in 1913, independently developed a similar model to describe the behavior of thermionic currents from filaments.¹⁶ In 1914, Townsend described the space charge influenced currents in terms of the mobilities of the charge carriers. It became common for the maximum currents, as allowed by the space charge, to be called space charge limited.^{12,11,10}

The concept of space charge has been used for a wide range of application. From the initial use for currents between charged plates, the space charge concept has been used in electronics for the design of tube-type electronic components,¹⁷ in meteorology to model lightning strikes, in aircraft design to evaluate charge buildup on various airplane structural components,⁹ in industry for the design and maintenance of electrostatic precipitators,¹⁸ and in the modelling of fields surrounding high voltage, direct current power transmission lines.¹⁷

As the field of mass spectroscopy developed, it was natural for the concept of space charge to be applied to the emerging technique. However, early workers correctly assumed that they were working with ion currents and ion densities that were too low for space charge to be important. The combinations of source conditions and ionization techniques being utilized made the modifications

of the Laplacian fields in the sources, by the space charge, insignificant.¹⁹

Recent years have seen a continual evolution of the mass spectroscopy field. New techniques for ionization have changed the conditions in the ionization source considerably. The atmospheric pressure ionization (API)⁵ and the electrospray ionization (ESI)⁷ techniques have utilized sources that have particularly deviated from the conventionally expected conditions of high vacuum and low ion densities. So, it can be argued that an assessment of the importance of space charge in the sources of some of these newer techniques is due. Notable in displaying the use of space charge analysis in high pressure mass spectrometry, is the ECD model by Gobby, Grimsrud and Warden.²⁰

Mathematical Background

To evaluate space charge effects in these newer sources, use of the previously developed methodology for determining space charge influenced fields must be made. However, early work with space charge was restricted to the analysis of simple geometries. Due to the difficulty of the mathematics involved, workers would idealize their experimental apparatus as either infinite parallel planes, concentric cylinders of infinite length, or concentric spheres.¹⁷ These geometries were amenable to mathematical analysis, yielding data appropriate to the individual

worker's needs. The computation of space charge influences in these geometries was based on the Poisson equation,

$$-\nabla \cdot \vec{E} = \frac{\rho}{\epsilon}, \quad (2)$$

where $\nabla \cdot \vec{E}$ is the gradient of the electric field, ρ is the space charge density in terms of charge per unit volume, and ϵ is electrical permittivity; and the continuity equation,

$$\left[\frac{\partial \rho}{\partial t} \right] + \nabla \cdot \vec{J} = 0, \quad (3)$$

where t is time. When considering stable ion source conditions, the steady state form of the continuity equation,

$$\nabla \cdot \vec{J} = 0, \quad (4)$$

can be used by assuming $(\partial \rho / \partial t) = 0$.

Here, $\vec{J}$ is the ion current density. As was discussed earlier, the ion current will have contributions from diffusion, convection, and electrostatic transport. This dependence of $\vec{J}$ can be mathematically stated as

$$\vec{J} = \kappa \rho \vec{E} - D \nabla \rho + \vec{F}, \quad (5)$$

where D is the diffusion constant and $\vec{F}$ is the gas flow vector. The first term relates to the ion drift contribution to the current density vector, while the second and third terms indicate the effects of diffusion and convection, respectively.¹⁰ Diffusion and convection terms

are important only in some very special situations, and are not treated in this work.

Beyond this point the mathematics will be expressed in scalar notation, instead of the previously used vector notation.

Analytic Solutions

For this work, the Poisson and continuity equations were utilized to predict electric fields, space charge densities, potentials, ion transit times, etc. for ion sources with certain assumed operating parameters. Given the wide variation in the geometries of real ion sources, all three simple geometries, amenable to giving analytical solutions, were considered. Similar analyses have previously been described, for use in discharge physics, by Townsend¹² and Chapman.²¹ Descriptions of these analyses, for each of the three geometries, follow.

Planar

In this geometry, shown in Figure 1, two planes of infinite area are placed parallel to each other at some finite distance, l . A potential difference, V_0 , exists between the two plates. A current, i , is assumed to flow between the two plates. Furthermore, all of this current is carried by one type of charged particle, with a mobility, κ . The unipolar current originates at one surface, and terminates at the other.

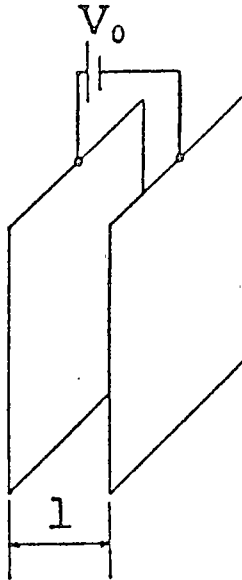


Figure 1. Planar Geometry, infinite parallel planes.

The mathematical analysis of the planar geometry gives electric field strength and ion density as a function of distance, x , from the source plate. A detailed derivation of the equations shown here is presented in Appendix A. The equations for field strength and space charge density are

$$E = \left(\frac{2i}{K \epsilon_0} x + E_0^2 \right)^{1/2} \quad (6)$$

$$\rho = \frac{i}{K} \left[\frac{2i}{K \epsilon_0} x + E_0^2 \right]^{1/2}. \quad (7)$$

Here E_0 is the field strength at the source plate ($x=0$). Graphs of the functions for certain sets of initial conditions are given in Figures 2, 3, 4, and 5. The Figures show the remarkable modification of the conditions in the source, in the space charge dominated (SCD) case. Especially noteworthy is the decrease in the electric field strength and the increase in the ion density in the area near the source plate.

Cylindrical

In this geometry, shown in Figure 6, a cylinder of radius, r_0 , is enclosed by a concentric cylinder of radius, r_1 . The surface of the inner cylinder acts to supply a current of charged particles that flow to the outer cylinder. These concentric cylinders are assumed to be of infinite length. Again, a potential difference exists between the two cylinders and the current is completely carried by charged particles of mobility, κ . The field strength is E_0 at the surface of the inner electrode ($r=r_0$).

The mathematical analysis of the cylindrical geometry gives electric field strength and ion density in terms of distance, r , from the axis at the center of the two

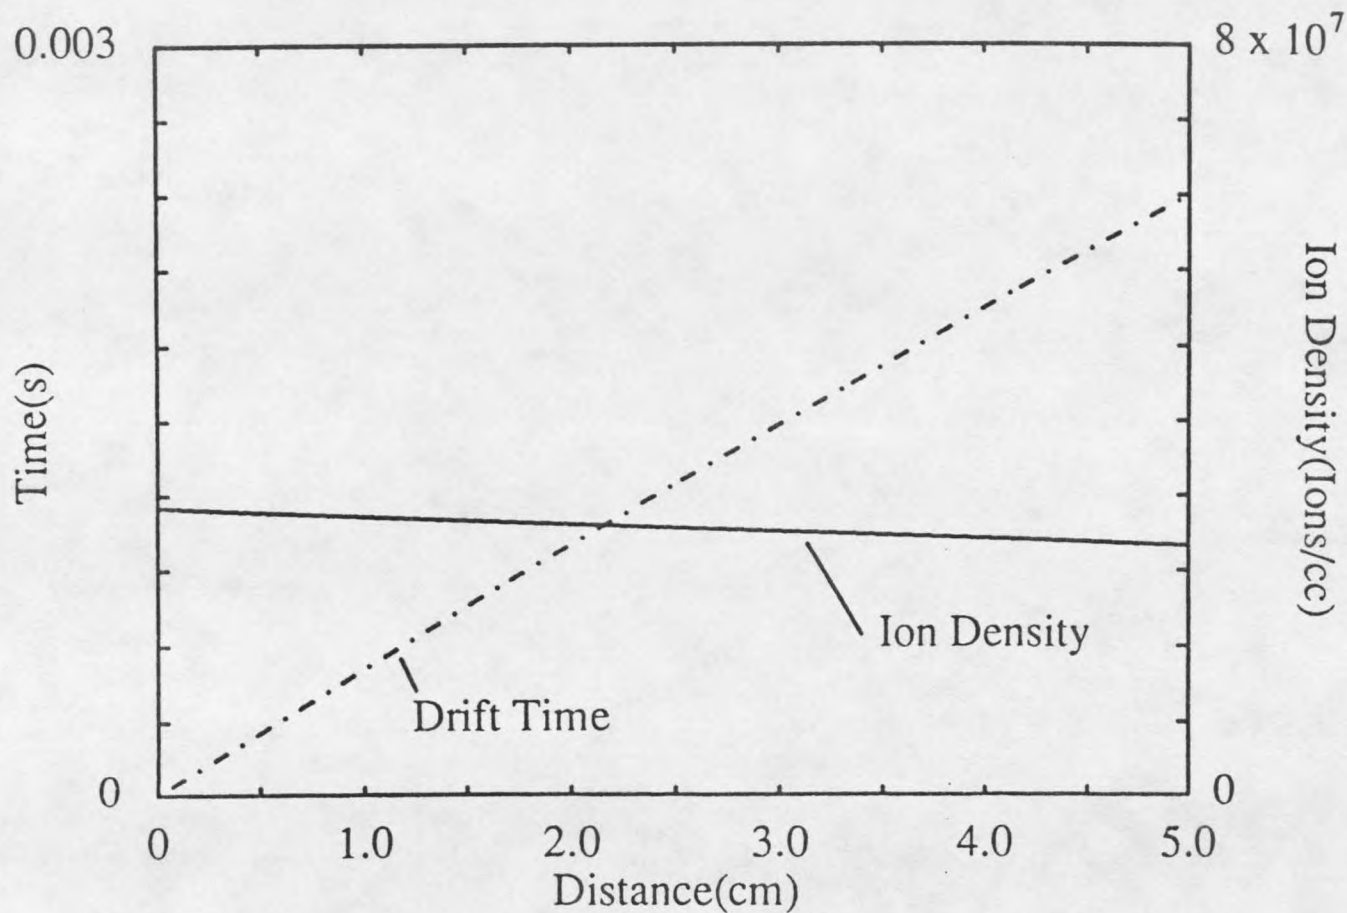


Figure 2. Non-space charge dominated residence times and space charge densities, in the planar geometry, as a function of distance. The current density is 1.0×10^{-8} A/cm²; the total applied potential, $V_0=10,000$ V; and the ion mobility, $\kappa=1 \times 10^{-4}$ m²/V·s.

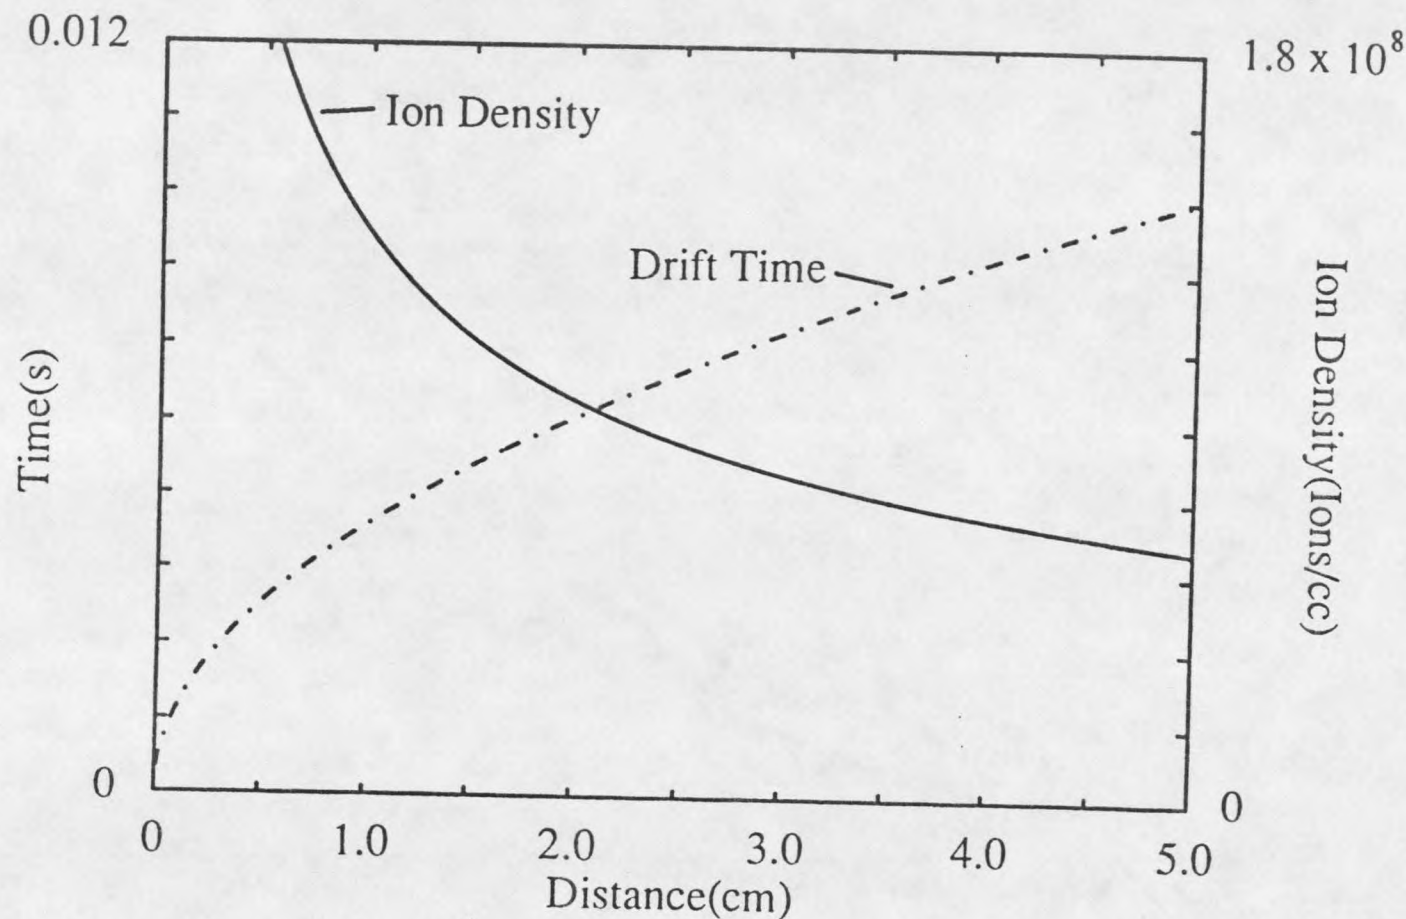


Figure 3. Space charge dominated residence times and space charge densities, in the planar geometry, as a function of position. The current density is 1.0×10^{-8} A/cm²; the applied potential, $V_0=3,600$ V; and the ion mobility, $\kappa=1 \times 10^{-4}$ m²/V·s.

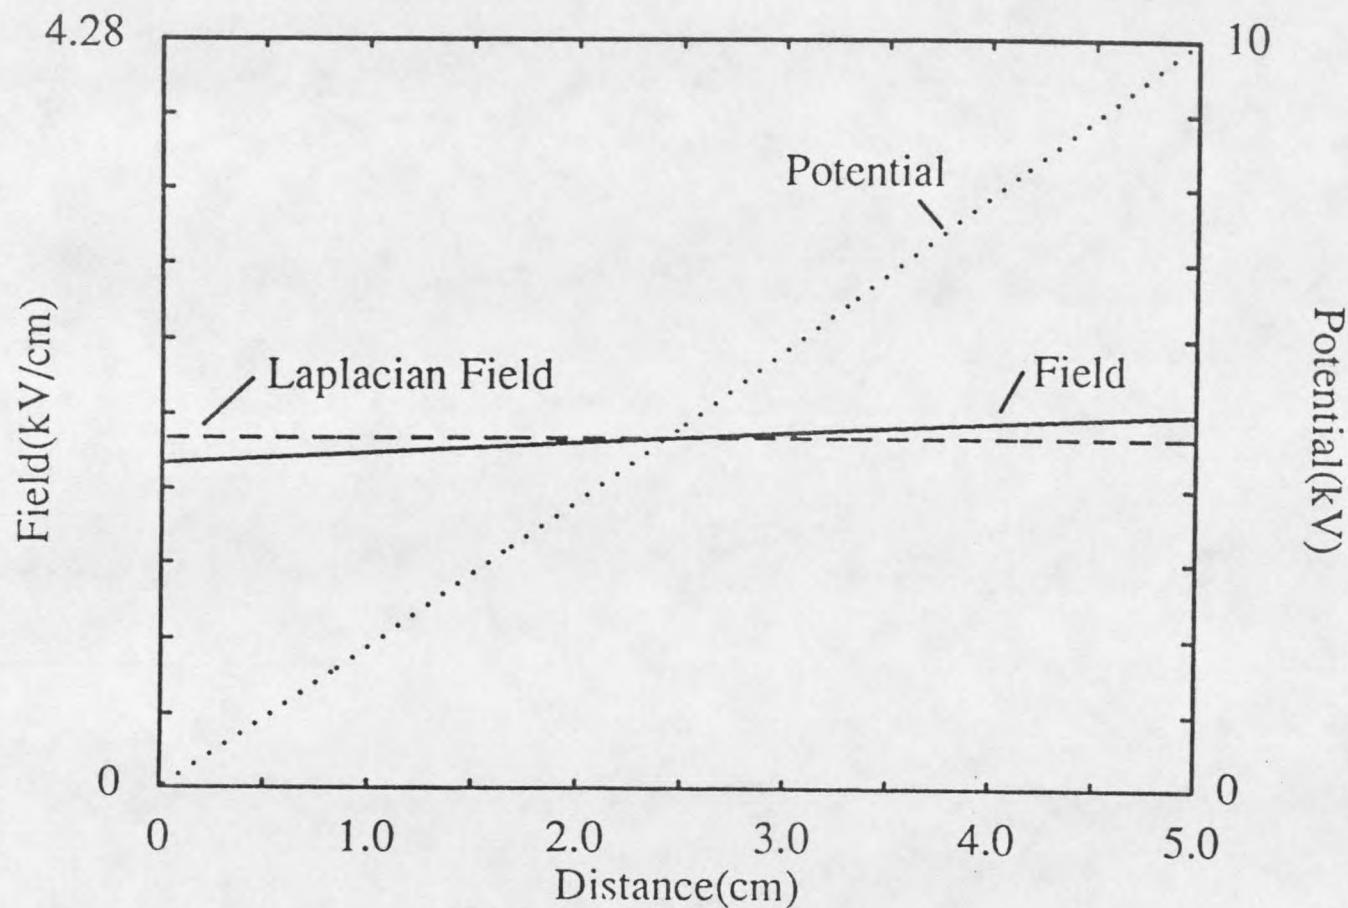


Figure 4. Non-space charge dominated potentials and fields, in the planar geometry, as a function of distance. Applied potential, current density, and ion mobility are as specified for Figure 2.

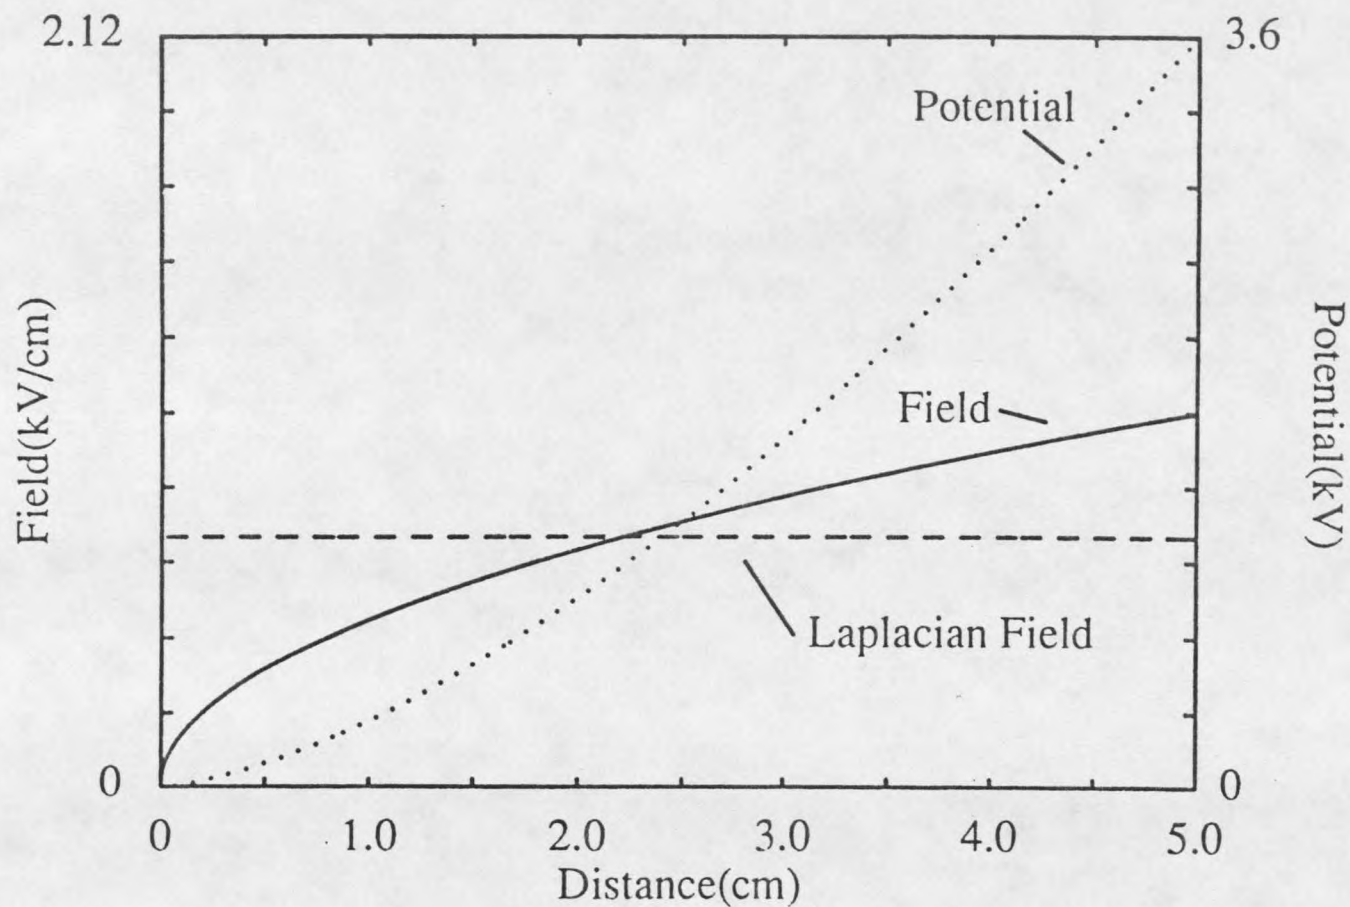


Figure 5. Space charge dominated potentials and fields, in the planar geometry, as a function of distance. Applied potential, ion current, and ion mobility are as specified for Figure 3.

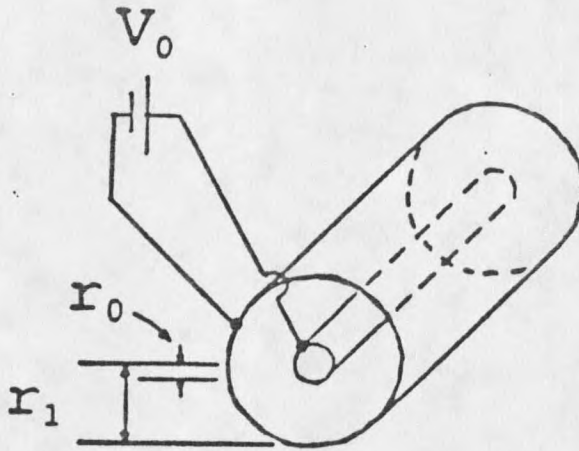


Figure 6. Cylindrical geometry, concentric cylinders of infinite length.

cylinders. Mathematically, the functions apply to the region between the concentric cylinders. A detailed derivation of the equations shown here is presented in Appendix A. The equations for field strength and space charge density are

$$E = \frac{r_0}{r} \left[\frac{i}{2\pi K \epsilon_0 r_0^2} (r^2 - r_0^2) + E_0^2 \right]^{1/2} \quad (8)$$

$$\rho = \frac{i}{2\pi r_0 K} \left[\frac{i}{2\pi K \epsilon_0 r_0^2} (r^2 - r_0^2) + E_0^2 \right]^{-1/2} \quad (9)$$

A graph of the functions for a certain set of initial conditions is given in Figures 7 and 8. Interestingly, in the space charge dominated case, the space charge density is independent of position. The cylindrical analysis was used by Shahin to model his cylindrical ion source. However, the dimensions of his source, as well as his low ion currents, made space charge influences negligible.¹⁹

Spherical

Analogous to the cylindrical case, this geometry, shown in Figure 9, involves concentric spheres. The inner sphere, which acts as an ion supply, is of radius, r_0 . The radius of the outer sphere is r_1 . The two spheres are separated by a potential difference, and current flows from the inner sphere to the outer sphere by the drift of charged particles of mobility, κ . The field strength is E_0 at the inner sphere surface ($r=r_0$).

The mathematical analysis of the spherical geometry gives field strength and ion density in terms of distance, r , from a point at the center of the two spheres. Mathematically, the functions are valid in the region between the concentric spheres. A detailed derivation of the

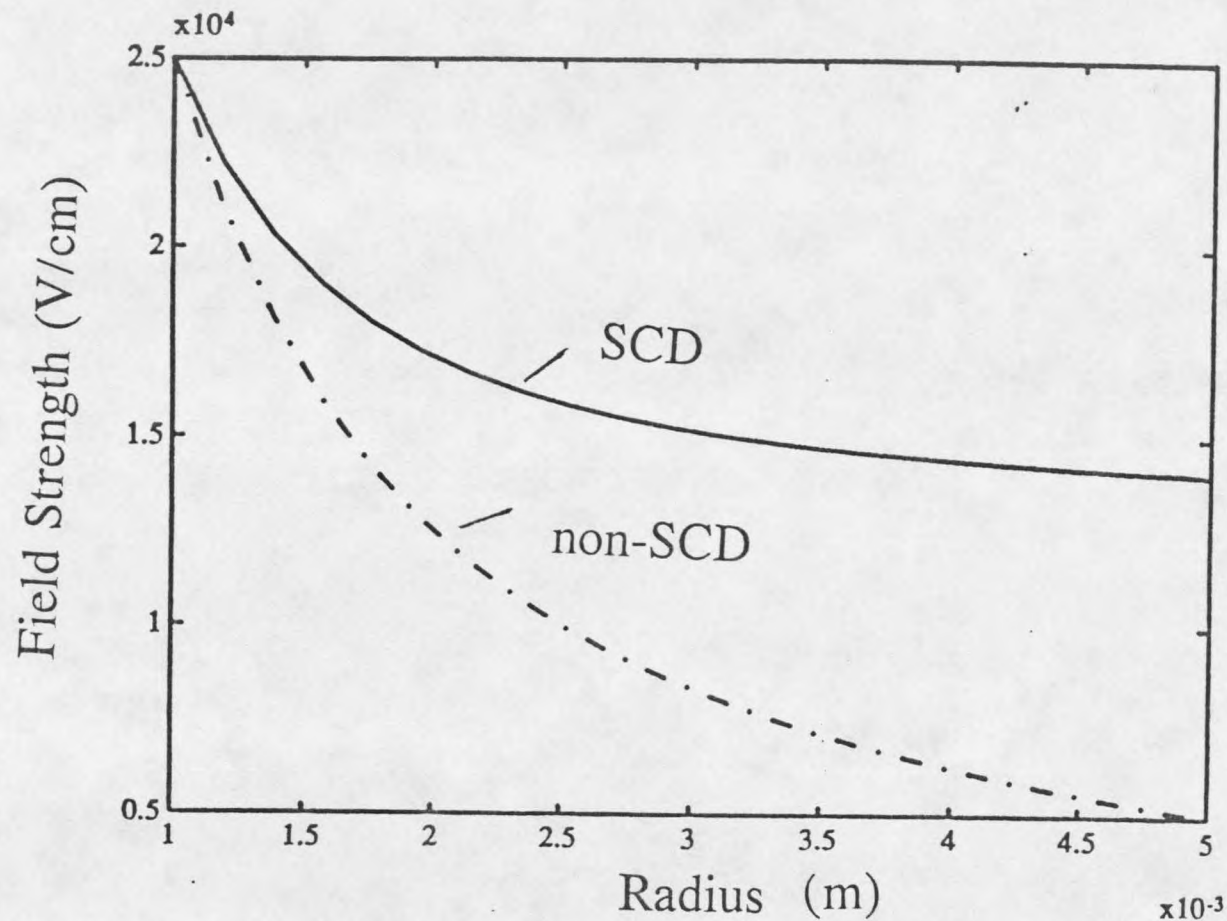


Figure 7. Fields with the consideration of space charge and without the consideration of space charge in the cylindrical geometry. The radii of the inner and outer cylinders are 0.001 and 0.005 m, respectively. The field at the inner cylinder surface, $E_0 = 2.5 \times 10^4$ V/m; the ion mobility, $\kappa = 1 \times 10^{-4}$ m²/V·s; and the ion current, $i = 1 \times 10^{-6}$ A/m.

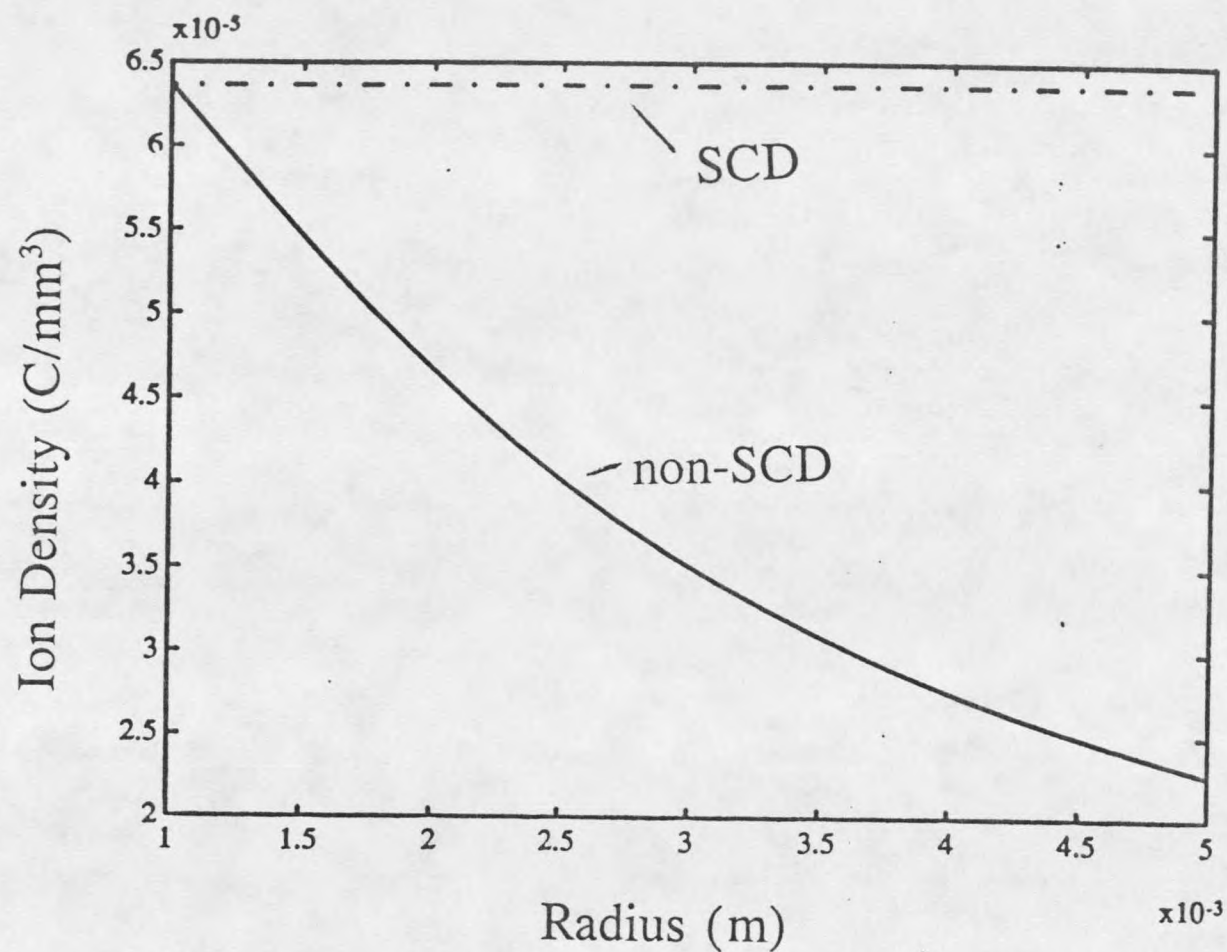


Figure 8. Space charge dominated and non-space charge dominated space charge densities in the cylindrical geometry. The conditions are the same as indicated for Figure 7.

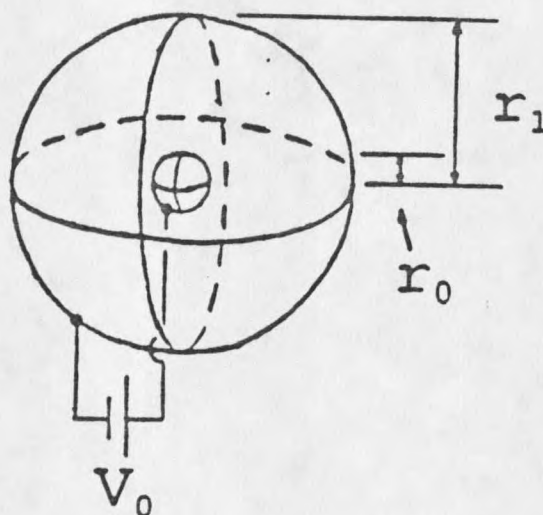


Figure 9. Spherical geometry, concentric spheres.

equations shown here is presented in Appendix A. The equations for field strength and space charge density are

$$E(r) = \left(\frac{r_0}{r} \right)^2 \left[\frac{i}{6\kappa\pi\epsilon_0 r_0^4} (r^3 - r_0^3) + E_0^2 \right]^{1/2} \quad (10)$$

$$\rho = \frac{i}{4\pi\epsilon_0 r_0^2 \kappa} \left(\frac{i}{6\pi\epsilon_0 \kappa r_0^4} (r^3 - r_0^3) + E_0^2 \right)^{-1/2} \quad (11)$$

A graph of the functions for a certain set of initial conditions is given in Figure 10. From the Figure it is evident that any analysis of such a space charge dominated source, without the consideration of space charge, would dramatically underestimate the actual field strength at distances far from the inner sphere surface.

Experimental work has been done, in the different geometries, to verify the equations. The cylindrical and planar geometries were experimentally studied by Child, Langmuir and Townsend at the time that the mathematical formulations were originally presented.^{15,16,12} Much later, Chapman produced similar experimental data to verify the description of the spherical model. Chapman measured the magnitude of space charge limited currents, and showed these currents to be in agreement with the analytic solutions²².

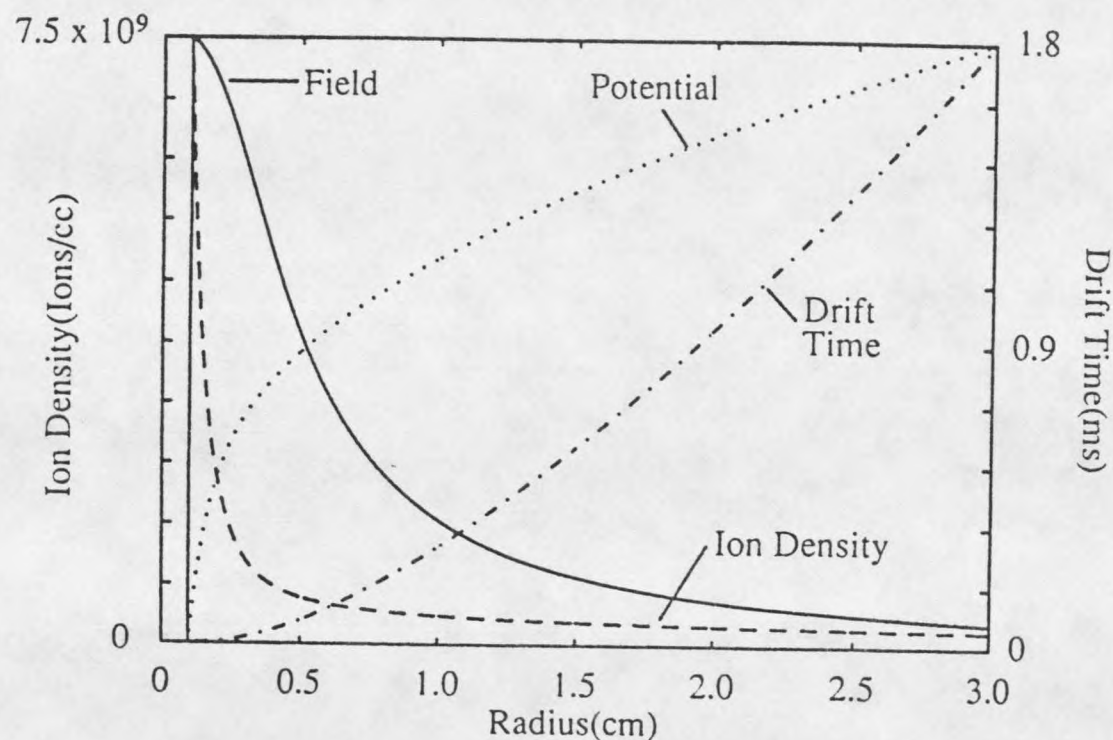


Figure 10. Space charge dominated conditions in the spherical geometry: Electric field potential, ion density and ion drift time for the space charge dominated case. The applied voltage, $V_0=7,693$ V; the supply surface radius, $r_0=0.1$ cm; the outer sphere radius, $r_{\text{out}}=3$ cm; the ion mobility, $\kappa=1 \times 10^{-4} \text{ m}^2/\text{V}\cdot\text{s}$; and the ion current, $i=6\mu\text{A}$.

APPLICATIONS OF THE ANALYTIC SOLUTIONS

The analytical solutions for the simple geometries presented in the previous section give at least a qualitative picture of what is happening in a actual ion source. There are two reasons why the models may not correspond directly to physical reality. First, they do not correspond precisely to the actual physical geometry of most sources. Second, they rely on a rather artificial distinction between the ionization and drift regions of the source, as will be discussed below. However, they do serve some instructive purpose. These models can be viewed as some crude approximation of actual source geometries. These models can give important insight into the perturbation of the Laplacian fields by space charge.

The spherical source, especially, can be used to model many ion sources. Many sources can be viewed as having a central ion source, and having walls, at least approximately equidistant, in all directions. This view gives the opportunity to evaluate a particular ion source with respect to some of its known operating parameters (i.e., potential and supply current). The data from this evaluation can give interesting information about the conditions inside the source. Especially important will be the way these

conditions will be influenced by the space charge density in the source. The data must then be assessed with respect to its dependence on the geometric approximations made in constructing the model.

Particularly useful pieces of information for an ion source are the ion residence time in the source, ion concentration at the sampling aperture and ion drift velocity at various locations in the source. Such information is readily available from this method of analysis, and is very interesting for a variety of applications, especially when the reaction kinetics for the drifting ions is important.

The ion source can be thought to be comprised of two rather arbitrarily divided regions; the ionization region and the drift region. When modelling the ion source by this method, the entire volume of the source is not being modelled. Instead, only the drift region is being considered. The ionization region will contain mechanisms that will produce ions, at its surface, at a given rate. Regardless of the ion source in question, processes of complexity beyond the scope of this study will occur in the ionization region. In the drift region, however, ions merely drift to the counter electrode. This reduces the source modelling into a much more workable problem.

The somewhat arbitrary division between the ionization region and the drift region has precedent.⁹ Much of

application of space charge theory is rooted in the study of corona discharges. A corona is used in the corona API source and is discussed below in that context. A corona discharge can be stimulated by biasing a needle with a large voltage. Events centered around the tip of the needle arise from the effect of the applied voltage on the air surrounding the needle. Many researchers observed light being emitted from the area immediately around the tip of the needle, at the center of a corona. This light emitting region was assumed to contain a plasma region, whereas the drift region was assumed to be on the outside of the light emitting region. The shape and size of the light emitting region was taken to be an indication of the shape and size of the plasma. This visual observation gave early researchers the justification for the division between the two regions.^{9,10,11} Shahin used a similarly arbitrary division for the analysis of his cylindrically symmetric corona mass spectrometer source.¹⁹

With mathematical models of the space charge influence in the simple geometries developed, attention can be turned to mass spectroscopic techniques utilizing sources in which space charge may have an important effect. Two of these techniques are Atmospheric Pressure Ionization (API) and Electrospray Ionization (ESI). Both of these techniques operate with relatively high source pressures and ion currents.^{11,7,6} Moreover, the drift region of each source is essentially unipolar.

Corona API in the Spherical Geometry

In the positive corona API source, shown in Figure 11, the ionization is caused by biasing a needle at a positive voltage high enough to initiate a corona. A detailed description of the processes involved in the corona has been provided by Loeb,¹⁰ Rees²³ and Sigmond.¹¹ Equations have been formulated to empirically model the behavior of the corona, immediately around the needle. An electron travelling in the corona will strike a number of neutral molecules causing an avalanche of electrons and, as a result, leaves positive ions. This primary ionization process corresponds to Townsend's primary ionization coefficient, α . A secondary ionization process, where ions are produced by collisions between molecules and the electrons produced in the avalanche, is described by a secondary Townsend ionization coefficient, γ . Through this complex regime of electron-molecule reactions, positive ions charge are driven outward, away from the needle tip. Similarly, negatively charged particles are attracted to the needle, and collected there.^{10,11}

Outside of a certain distance from the needle tip, only particles of a charge being the same as the needle's will exist. This region, away from the needle tip, can be considered to be the drift region. In this drift region, the only process occurring is the motion of the ions, through ion drift.

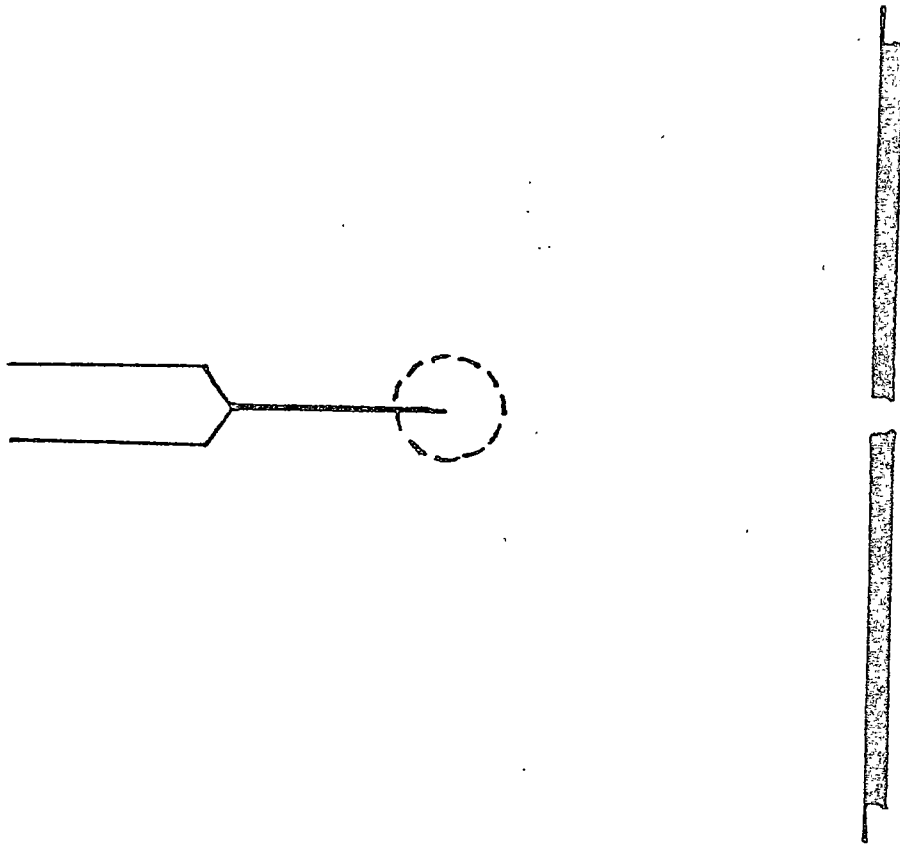


Figure 11. Schematic of the corona API.

Using the spherical geometry as a model for the API source, one can model the ion motion in the drift region. First, the ionization region of the source must be made to conform to the developed model. The ionization region can be reduced simply to a spherical ion supply surface, the inner sphere in the spherical model. The idea of the spherically symmetric ion supply surface has been supported by analysis of photographs of the plasma regions surrounding corona needles.⁹ This ion supply surface will produce an ion current uniformly over its entire surface area. The ion

current will consist of ions having a mobility, κ . According to tabulated data of ion mobilities, most ions in an API source will have a mobility of about $1 \times 10^{-4} \text{ m}^2/\text{V}\cdot\text{s}$.¹³

Here, a problem with the entire modelling process must be faced. The solution to the derived equations for the spherical model is dependent on boundary conditions. These boundary conditions are values of important conditions on the boundaries of the region to be modelled. Especially important are the conditions on the ion supply surface. Since the modelling of the ionization processes in the corona, or in terms of the model, the conditions at the supply surface, are beyond the scope of this study, the problem of deciding appropriate parameters for this model becomes especially difficult. It was decided to model the API source with the ability to specify E_0 , the field strength at the ion supply surface. E_0 was varied over a wide range of values and then the entire range of results was evaluated. Figure 12 shows results, in terms of E , ρ , t and V , of modelling the API over a range of E_0 values. As is demonstrated in the Figure, the choice of E at the inner boundary of the drift region does not greatly influence conditions, except for potential, further out in the drift region.

The parameters used in the model are κ , r_0 , I_0 , and E_0 . For the Figure, $\kappa = 1 \times 10^{-4} \text{ m}^2/\text{V}$, $r_0 = 0.03 \text{ m}$ and $I_0 = 6 \text{ } \mu\text{A}$ were used. Six different choices for E_0 were used: 40, 35,


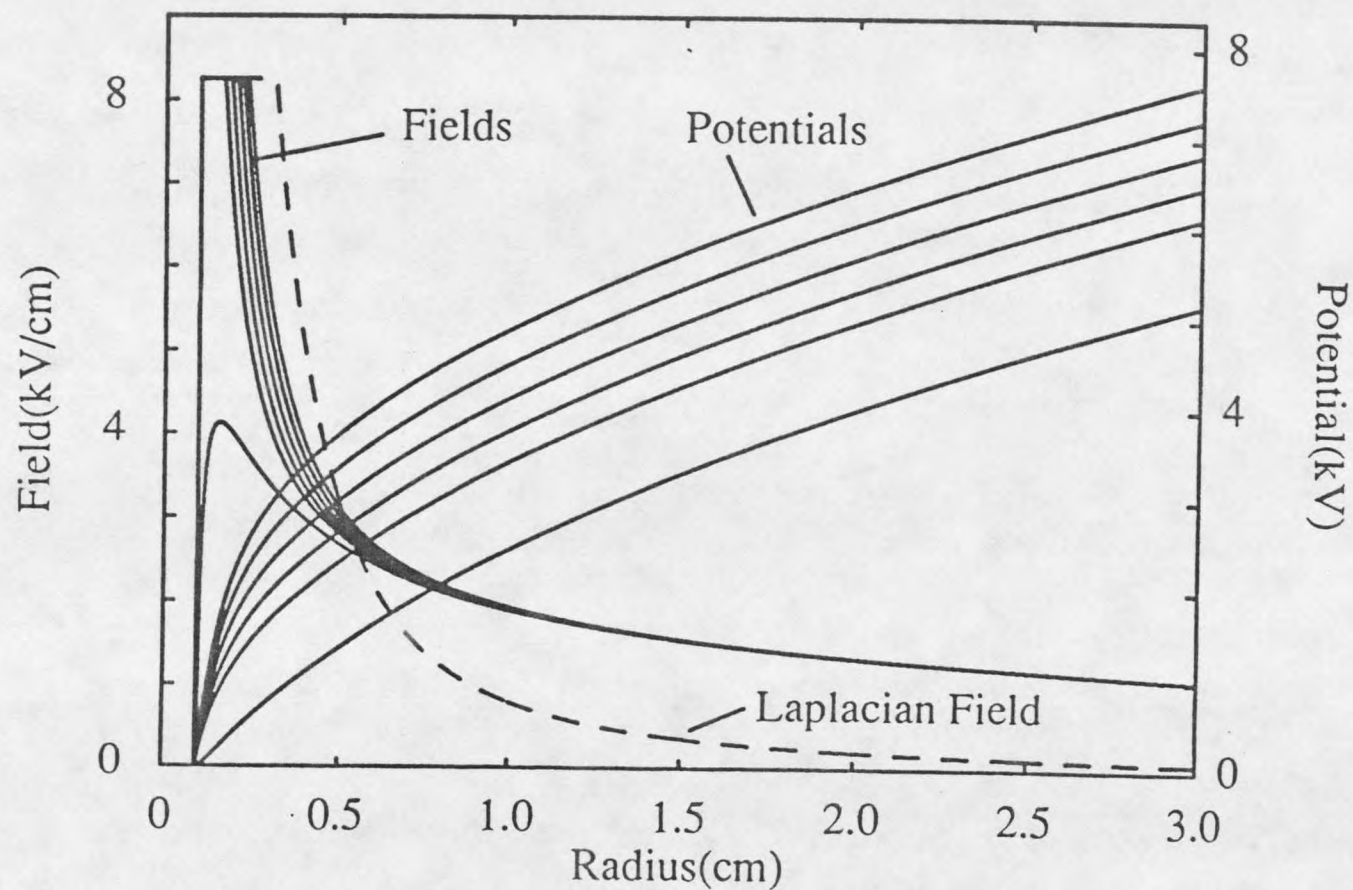


Figure 12. Conditions in the corona-API source: Field strengths and potential distributions versus radius for 6 different values of applied potential.

30, 25, 20, and 0 kV/cm. As is apparent in the figure, only in the area near the ion supply surface is the effect of the choice of E_0 important. The comparison of the Laplacian field curve and the other curves, for actual electric fields, makes obvious the important effect that space charge plays in this system. The space charge domination serves to coalesce the field strengths in the outer area of the spherical source.

In the corona API source, the analyte molecules are usually not directly ionized by the corona. Instead, the ions supplied from the corona are largely reagent ions. These reagent ions result from the ionization of some of the neutral gas molecules present in the source. Often the ions in the source are hydrated hydronium ions, $H_3O^+(H_2O)_n$. The analyte molecules are of much lower concentration than those of the reagent gas. The reagent ions will, in turn, react with the traces of analyte molecules present in the source, often in a reaction of the type:



where B is an analyte molecule. The extent of analyte ionization, and thus sensitivity, will depend on the time that it takes for the reagent ions to transit the gap between the ion supply surface and the sampling orifice on the outer wall of the source. Hence, it becomes important to

know the residence time, t_{res} for the reagent ions in the source. It is necessary to know the residence time in order to properly evaluate the kinetic data acquired in corona API experiments.

Approximate expressions for ion transit times, along with other interesting source parameters, have been derived from the spherical geometry solutions. For a space charge limited source with the ion supply surface radius, r_0 , being much smaller than the outside surface radius, r_1 , expressions for ion residence time, t_{res} ; sample ion density, ρ_{samp} ; and applied potential, V_d can be written.

$$t_{\text{res}} = \left[\frac{8\pi\epsilon r_1^3}{3K i} \right]^{1/2} \quad (13)$$

$$\rho_{\text{samp}} = \left[\frac{3\epsilon i}{8\pi K r_1^3} \right]^{1/2} \quad (14)$$

$$V_d = \left[\frac{2i r_1}{3\pi K \epsilon} \right]^{1/2} \quad (15)$$

Derivations of these equations are shown in Appendix B. The

equations are graphed, over a certain range of time, in Figure 13.

Electrospray in the Spherical Model

Likewise, the Electrospray (ESP) source, shown in Figure 14, can be analyzed by the spherical space charge model. Similar problems with choices of parameters, relating to boundary conditions, exist in this model. In the ESP source the analyte is introduced into the ion source by injecting a stream of a volatile liquid, containing a small concentration of analyte molecules, through a hypodermic needle. The needle is put at high voltage with respect to the rest of the ion source. As the stream of liquid exits the tip of the needle, it becomes charged and starts to break into droplets. The droplets each carry a charge of the same sign as the charge on the needle. Even though the dynamics of charged droplets, such as these, have been studied since the time of Lord Rayleigh, the exact mechanisms involved in the behavior of these droplets are still not well understood. However, through the work of Vestal,⁶ Dole,⁷ Iribarne and Thomson,²⁴ a general scheme for ion production has been developed. As a droplet travels further away from the needle, it is observed that both ions and solvent molecules evaporate from the droplet's surface. Several effects combine to determine the course of the droplet's reduction in size. Surface tension will tend to

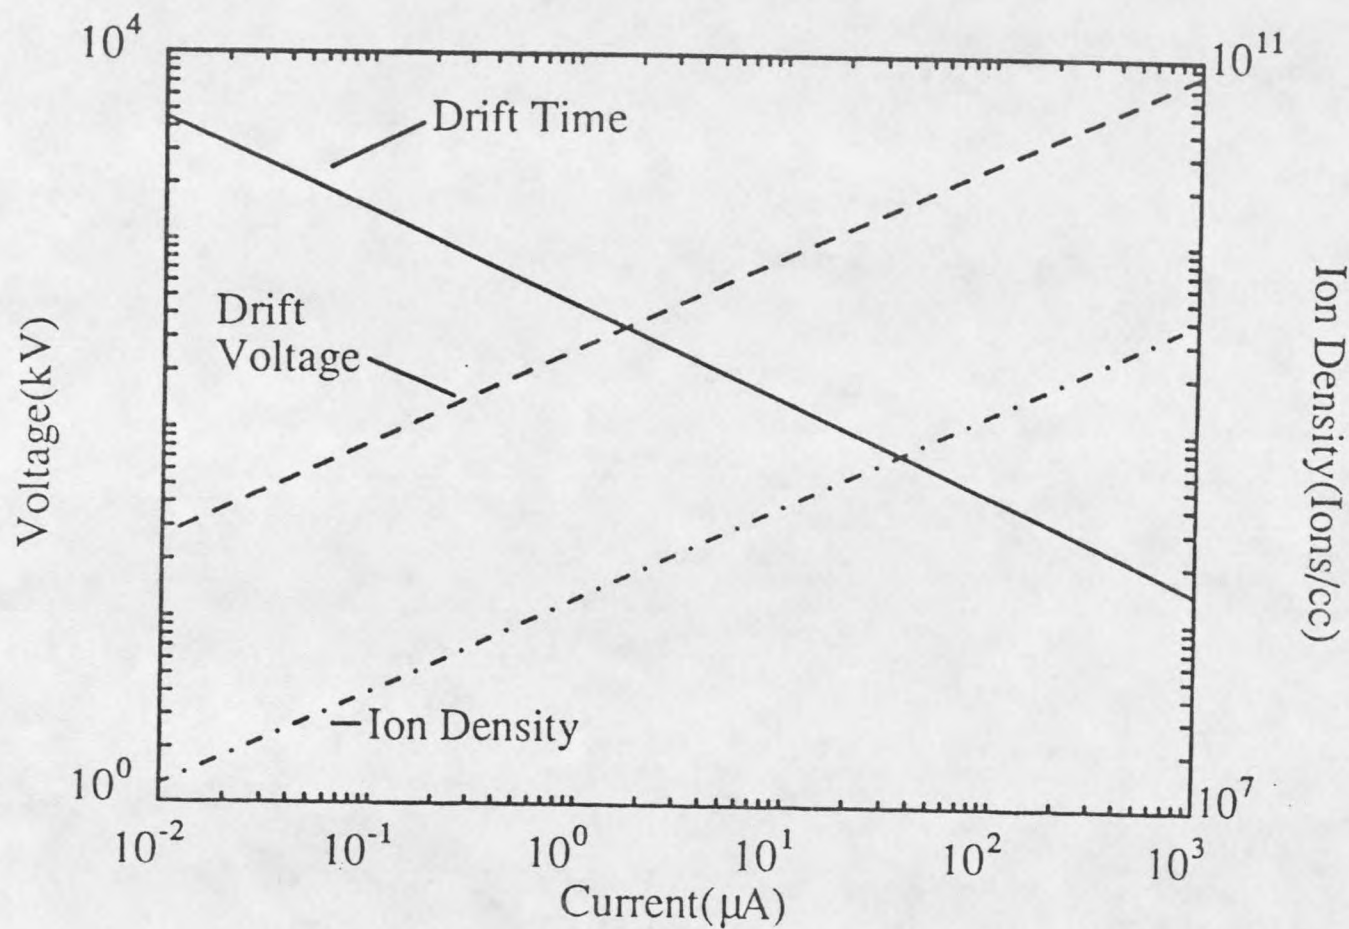


Figure 13. Variation of residence time, potential distribution and ion density with discharge current in the spherical ion source geometry. The conditions are as specified in Figure 10.

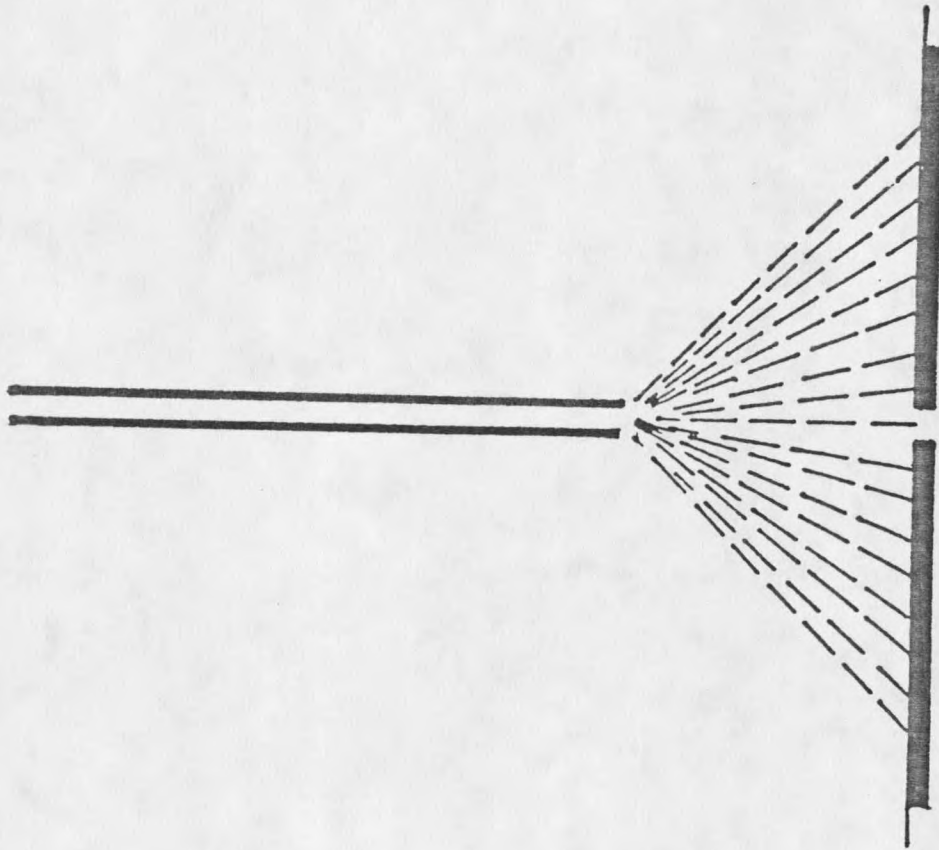


Figure 14. Schematic of the Electrospray.

keep the droplet's surface intact. This will restrict the droplet's contained liquid to a certain volume. Coulombic repulsions will tend to keep the carriers of the droplet's charge separated as far as possible, and therefore, near the droplet's surface. The energy in the system will cause neutrals to evaporate from the surface of the droplet. As the droplet's size reduces, the coulombic repulsive forces will overcome the surface tension and cause the droplet to split into two or more droplets thus reducing the crucial parameter for the coulombic forces, charge per surface area.

Further solvent evaporation will cause the cycle of evaporation and droplet splitting for the droplets to continue, until the droplets become very small. At some time during this cycle of events, ions may evaporate from the surface of a charged droplet taking some or all of the droplet's charge with them.⁶ The production of a wide range of both sizes and charges of ions has been noticed. Charges as high as 1000, as well as masses up to 2,000,000 daltons have been reported.⁷

It is apparent that droplets of varying radii and charge are involved in the production of an ion current at a sampling orifice. The range of charges and masses involved spans a wide range of ion mobilities. To predict the response of the larger droplets to the convective, as well as electrostatic, forces acting in the source would be a difficult task. However, making the simplification of equating the area immediately around the capillary tip with a spherical ion supply surface and assuming all of the ions in the drift region to be of equal charge and mobility, makes the analysis easily possible. Although much mechanistic detail is sacrificed with the model, the information available from the simple analysis gives some interesting and useful information.

Using equation 14, the degree of space charge influence can be calculated. Using a needle to orifice distance of 5 cm, a ion mobility value of $1 \times 10^{-4} \text{ m}^2/\text{V s}$, and an ion

current of 10^{-6} A, the space charge potential is about 3500 V. This potential is in the range of the applied voltage used in the operation of the electrospray source. Therefore the electrospray source is strongly space charge influenced, if not dominated.

By this construction of an electrospray model, the model becomes essentially identical to the previously discussed API model. The operating parameters used in the API model are appropriate for the normal range of ESP operating parameters. From Figure 12, the illustration of the API modelling, it is apparent that the ESP source, as modelled, is also strongly space charge influenced. The areas distant from the hypodermic needle tip are relatively unaffected by the changes of E_0 at the ion supply surface. However, in a recent paper ion drift times were calculated using the Laplacian electric field.²⁵ Clearly, such analyses will be substantially in error.

GENERAL GEOMETRIES

The extension of the mobility model of ion transport to more general geometries requires a mathematical approach that can be applied to these general geometries. One possible approach to generalizing the technique is to use numerical methods to solve the same differential equations that were solved analytically for the simple geometries. Another approach would be to take some observations from the simple solutions, and to generalize them without explicitly calculating the electric fields at every point in an ion source. Both approaches will be discussed here, with the latter generalization being pursued first.

Unipolar Charge Drift Formula

The solution to the cylindrical model has been extended into a form that can be applied to more general geometries. The unipolar charge drift formula,

$$\frac{1}{\rho(t)} - \frac{1}{\rho_0} = \frac{\kappa}{\epsilon_0} (t - t_0), \quad (16)$$

provides space charge densities, for unipolar currents, without requiring any explicit knowledge of the source

geometry. Here $\rho(t)$ is space charge density as a function of time, t . ρ_0 and t_0 are the initial space charge and time, respectively. This equation is useful for estimating the space charge effect in almost any system. The natural tendency of ions is to spread out, by nature of their coulombic repulsions. It must be cautioned that, although the formula is geometry independent, it is dependent on the ion flow being unipolar.

All that is needed to apply this formula is an initial space charge and the time required to travel from the initial point to the point in question. Regardless of the application, the formula will describe the gradual broadening of a cloud of charge, as it drifts.¹¹ The application of the formula to three different initial space charge densities is shown in Figure 15. Interestingly, the ion densities converge at the long drift times.

An important consequence of the unipolar drift formula is that it is impossible to "squeeze" space charge closer together. A source cannot be constructed that will increase the concentration of ions in a dilute volume of space charge. The futility of efforts to "focus" ions is apparent in the simplicity of this equation. The equation is totally independent of applied fields. According to the formula, the only way to increase the sampled concentration of ions is to reduce the time between the creation of the ion density and their sampling. This situation has been reinforced by the

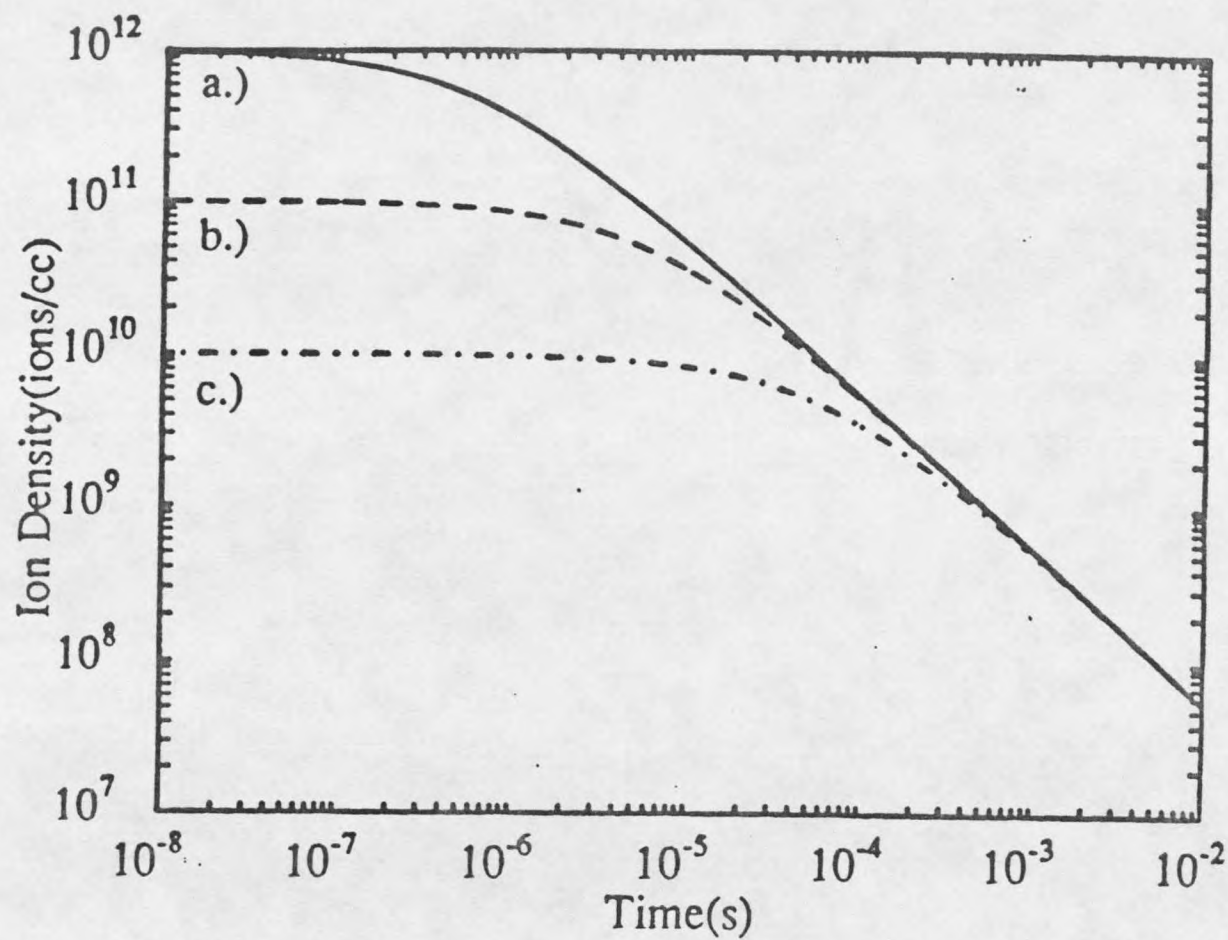


Figure 15. Ion density versus time in a unipolar ion source for three different values of ρ_0 , the ion density at $t=0$, calculated for the unipolar drift formula.

use of a simulation.^{26,27} In this simulation, a high potential was applied to the walls of a source, in an attempt to "squeeze" ions together. Figures 16, 17, 18 and 19 show the field and ion density contours for the simulation with, and without, the application of the focussing potential. While the ion density contour lines seem to be concentrated toward the sampling aperture, the sampled ion density actually goes down. The applied potential has actually slowed ion flow, and consequently increased the time for the ion density to spread. Further indication of this reduction in sampled ion density is given in Figures 20 and 21, where the focussed and unfocussed ion densities and ion currents are given.

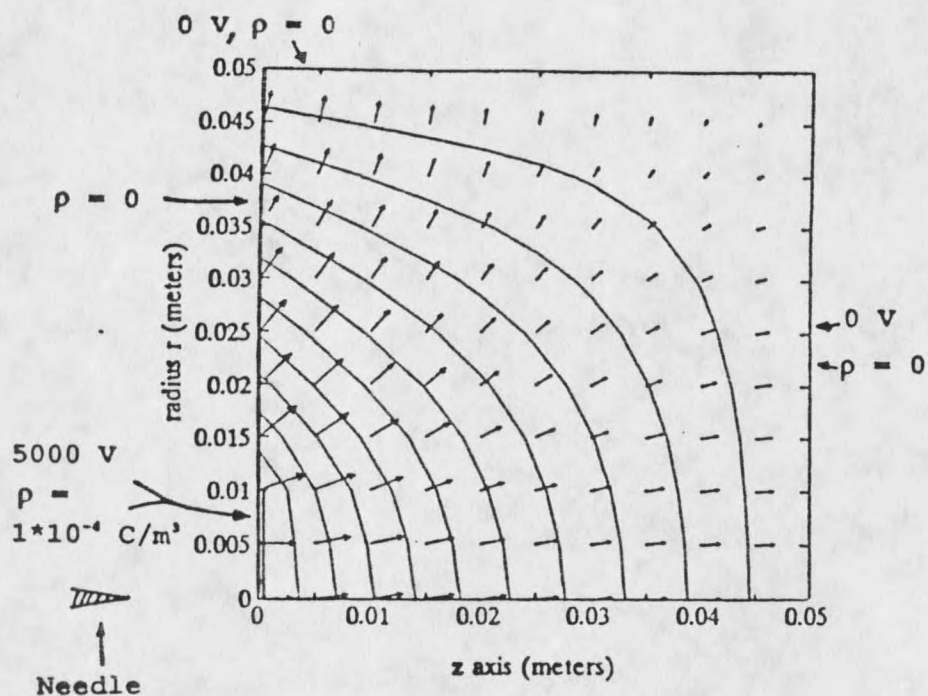


Figure 16. Case 1: Potential and field contour.

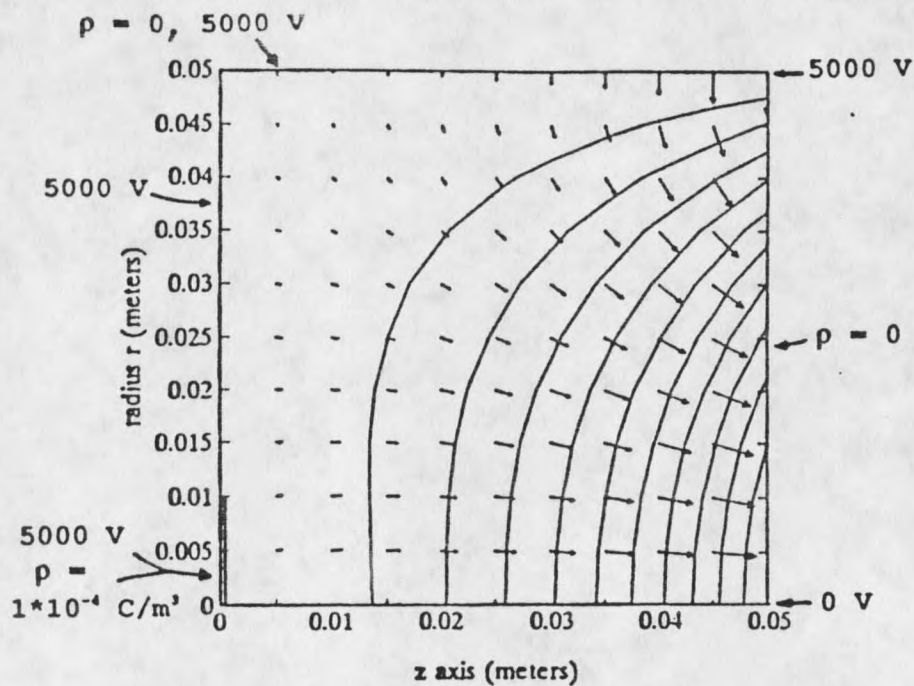


Figure 17. Case 2: Potential and field contour.

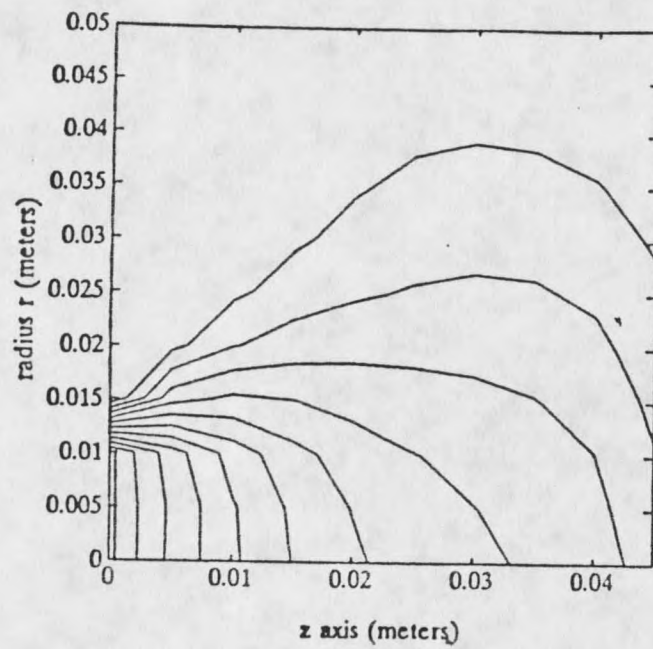


Figure 18. Case 1: Charge density contour.

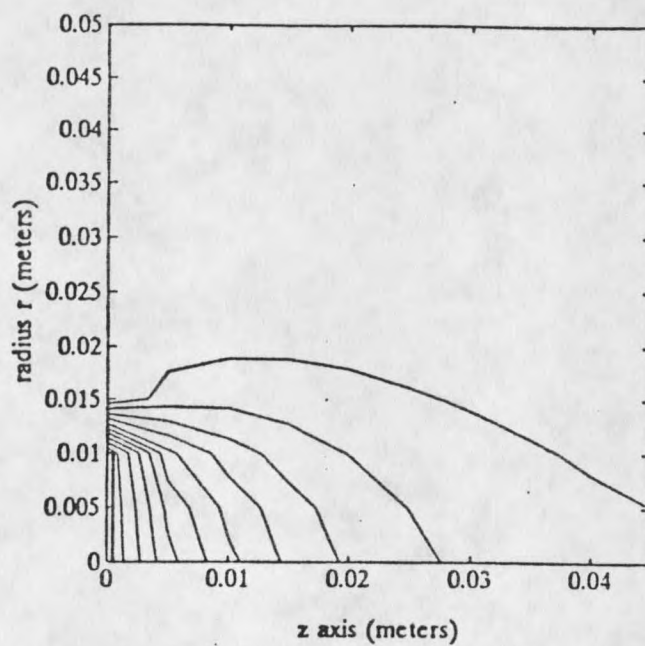


Figure 19. Case 2: Charge density contour.

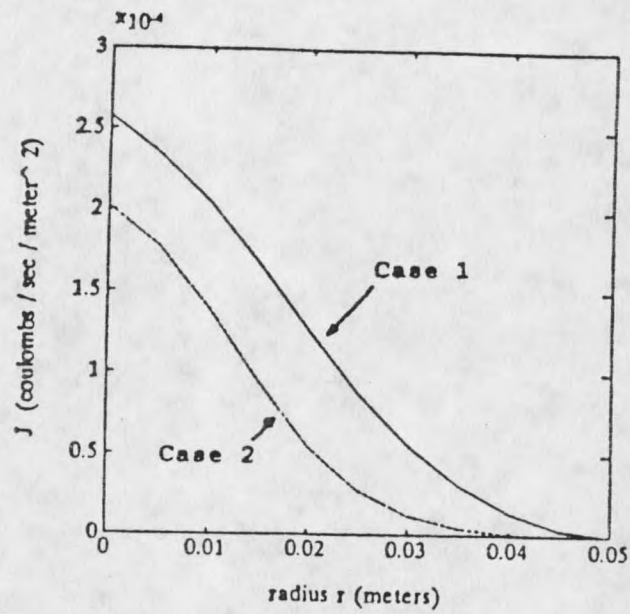


Figure 20. Current density vs. radius.

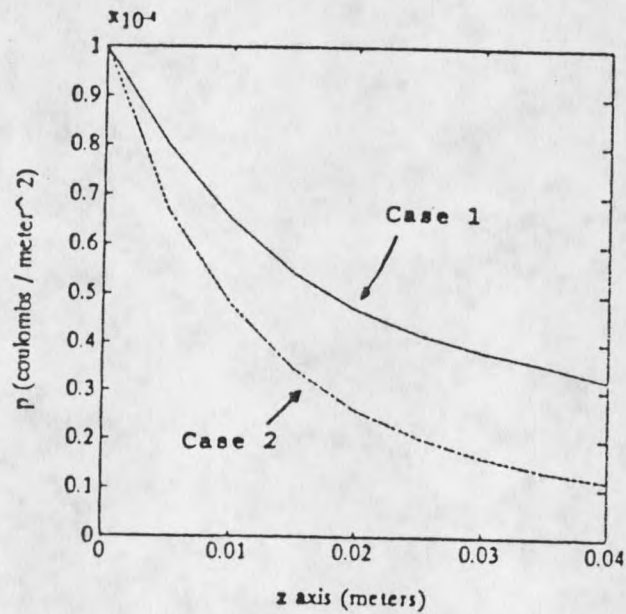


Figure 21. Charge density vs. radius.

Calculation of Absolute Sensitivities

The spherical ion source model is adequate for rough estimates of residence times for ions that would allow kinetically controlled processes to occur during ion transport. An example of this utility is the use of the unipolar formula for the evaluation of kinetically controlled ion molecule reactions.

One can assume a model for the kinetically controlled ion source. The ion supply surface supplies only one type of ion, a reagent ion, R^+ . This ion can react with a molecule, P . The reaction between these two species is second order. The molecule, P , is the analyte molecule of interest, and therefore, the ion current of the analyte ion, P^+ , can be modelled on the basis of the transport and reaction processes occurring in the source. The second order reaction is,



with the reaction having a second order rate constant k_1 .

Because the source is at high pressure, the ion densities will be small, as compared to the neutral densities. This condition allows the kinetics to be evaluated as being pseudo-first order. Putting the kinetics in terms of the concentration of the reagent ion concentration gives

$$\frac{d[R^+]}{dt} = k_1[R^+][P], \quad (18)$$

or in terms of pseudo-first order kinetics

$$\frac{d[R^+]}{dt} = k'_1[R^+], \quad (19)$$

where the pseudo rate constant is

$$k'_1 = k_1[P]. \quad (20)$$

Rearranging the pseudo-first order rate equation into an integratable form gives

$$\frac{d[R^+]}{[R^+]} = -k'_1 dt, \quad (21)$$

which upon integration gives

$$\ln[R^+] - \ln[R^+]_0 = -k'_1(t - t_0). \quad (22)$$

Assuming $t_0 = 0$ gives

$$\ln[R^+] = -k'_1 t + \ln[R^+]_0 \quad (23)$$

or

$$[R^+] = e^{(-k'_1 t + \ln[R^+]_0)} = [R^+]_0 e^{(-k'_1 t)}. \quad (24)$$

Upon substituting for the pseudo-first order rate constant, the reagent ion concentration is given as

$$[R^+] = [R^+]_0 e^{(-k_1[P]t)}. \quad (25)$$

The current, I , exiting an orifice in the source would be the product of the space charge density, ρ , and the ventilation rate, S , at the orifice aperture

$$I = \rho \cdot S. \quad (26)$$

The current, I , is composed of charged species passing through the orifice. In this case it would be composed of ions R^+ and P^+ . To produce an expression for the analyte ion current would require a ratio of analyte ion density to total ion density. This ratio, multiplied by the total current at the orifice, would give the analyte current at the orifice. The analyte current, I_{p^+} , would be:

$$I_{p^+} = \rho \cdot S \cdot \frac{\text{analyte ion concentration}}{\text{total ion concentration}}. \quad (27)$$

Here, the total ion concentration would be the sum of the reagent and analyte ion concentrations, which would, in turn, be equal to the initial ion concentration:

$$\text{total ion concentration} = [R^+] + [P^+] = [R^+]_0. \quad (28)$$

The analyte ion concentration would be the reagent ion

concentration subtracted from the initial reagent ion concentration:

$$\text{analyte ion concentration} = [P^+] = [R^+]_0 - [R^+]. \quad (29)$$

From the above kinetic argument, the ratio of analyte ion concentration to total ion concentration would be:

$$\frac{\text{analyte ion concentration}}{\text{total ion concentration}} = \frac{[P^+]}{[R^+] + [P^+]} \quad (30)$$

$$= \frac{[R^+]_0 - [R^+]}{[R^+]_0} \quad (31)$$

$$= 1 - e^{-k_1 [P] t} \quad (32)$$

$$= \frac{[R^+]_0 - [R^+]_0 e^{-k_1 [P] t}}{[R^+]_0} \quad (33)$$

Substitution of this expression into the equation for analyte ion concentration gives:

$$I_{p^+} = \rho \cdot S \cdot \left(1 - e^{(-k_1 [P] t)} \right) \quad (34)$$

This equation can be used to model the analyte ion current in a spherical ion source, that is operated with conditions similar to typical corona-API sources. The implications of this relationship are illustrated in Figure 22, where analyte ion current is plotted against ion drift time. The curves correspond to a variety of initial reagent ion and analyte molecule concentrations. The maxima in the curves result from two competing processes. First, the ion-molecule reaction will produce analyte ion concentrations that will increase with time. Second, the space charge expansion will cause the total ion concentration, and thus the analyte ion concentration, to decrease. The canceling effect, that these processes have on each other, produces the broad maxima found in Figure 22. For curve e, in Figure 22, a 4mm depth of a curtain gas was included. The other conditions were the same as in curve c. The curtain gas is a current of gas flowing in front of the sampling aperture. It is often composed of dry nitrogen, and serves to decluster the analyte molecules as they exit the ion source. Here, the curtain gas serves to end the region where reactivity is possible, but the unipolar expansion will continue as the ions continue to drift toward the orifice. The x-coordinate for distance was calculated from equation 13, the equation

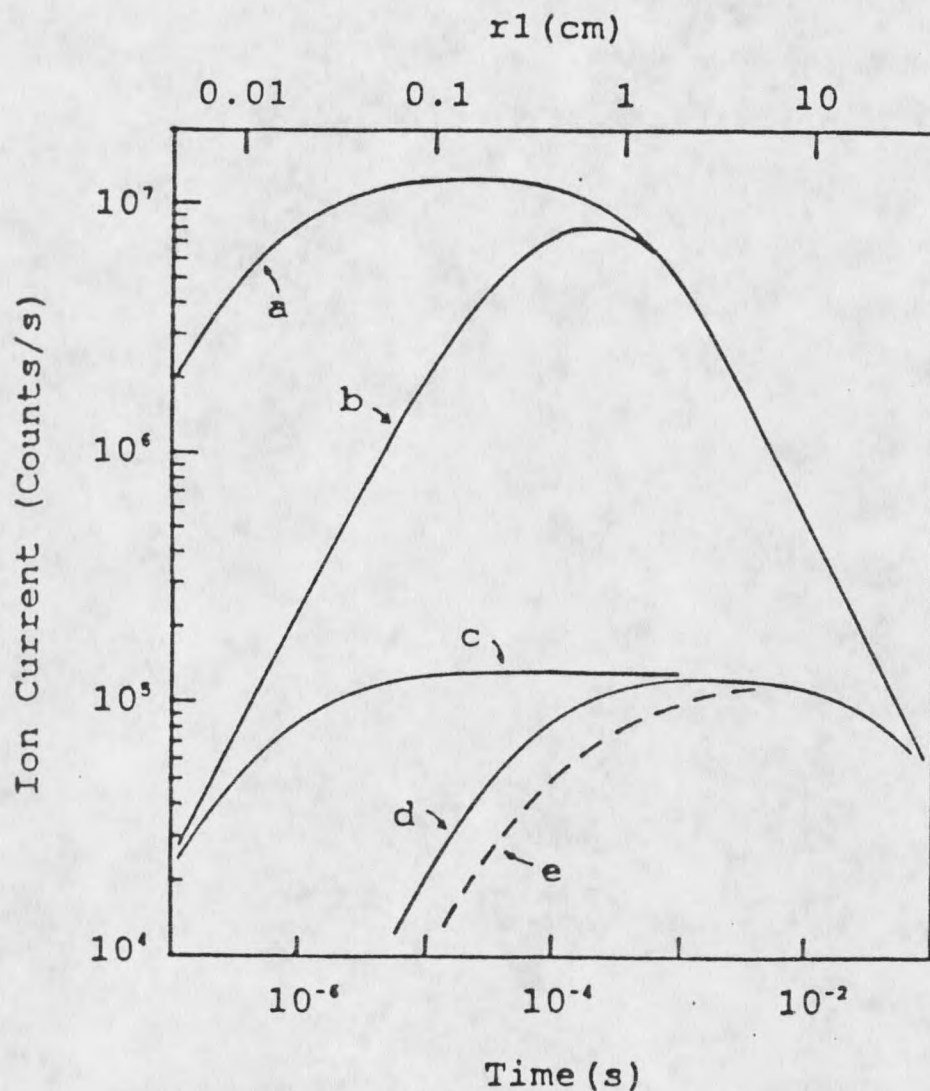


Figure 22. Kinetically influenced corona API ion currents: analyte ion intensities in a corona API source versus ion drift time. The upper x-axis shows needle to orifice distance for a discharge current of $3\mu\text{A}$. The curves correspond to: a.) $\rho_0=10^{12}$ ions/ cm^3 , c_a (analyte concentration)=100 ppb; b.) $\rho_0=10^{10}$ ions/ cm^3 , c_a =100 ppb; c.) $\rho_0=10^{12}$ ions/ cm^3 , c_a =1 ppb; d.) $\rho_0=10^{10}$ ions/ cm^3 , c_a =100 ppb; and e.) same as c.) but with 4mm of curtain gas in front of the orifice.

for ion residence time in the limiting condition of space charge domination. A current of $3\mu\text{A}$ was used for the calculation.

This methodology can be compared to experimental results for such a system. Figure 23 shows calculated analyte intensities as a function of distance between the source needle and the sampling orifice. The analyte, pyridine, was assumed to have a rate constant, $k=2 \times 10^{-9} \text{ cm}^3/\text{molec/s}$ in ambient air. The pyridine was present at a concentration of 0.1 ppb. Included in the model was a 4 mm depth of a curtain gas. Figure 24 shows the corresponding experimental result.²⁸

This model gives insight into the factors determining the absolute ion current at a sampling orifice. Prior to this work there was little understanding of these factors.

Numeric Solutions

In mathematics, alternatives to analytic methods for solving differential equations have been developed. The field of numerical methods of differential equations has provided methodologies for solving different classes of differential equations. These methods, in general, involve a discretization of a mathematical region. The differential equations are then mapped over the discretized region. This necessitates the transformation of the differential

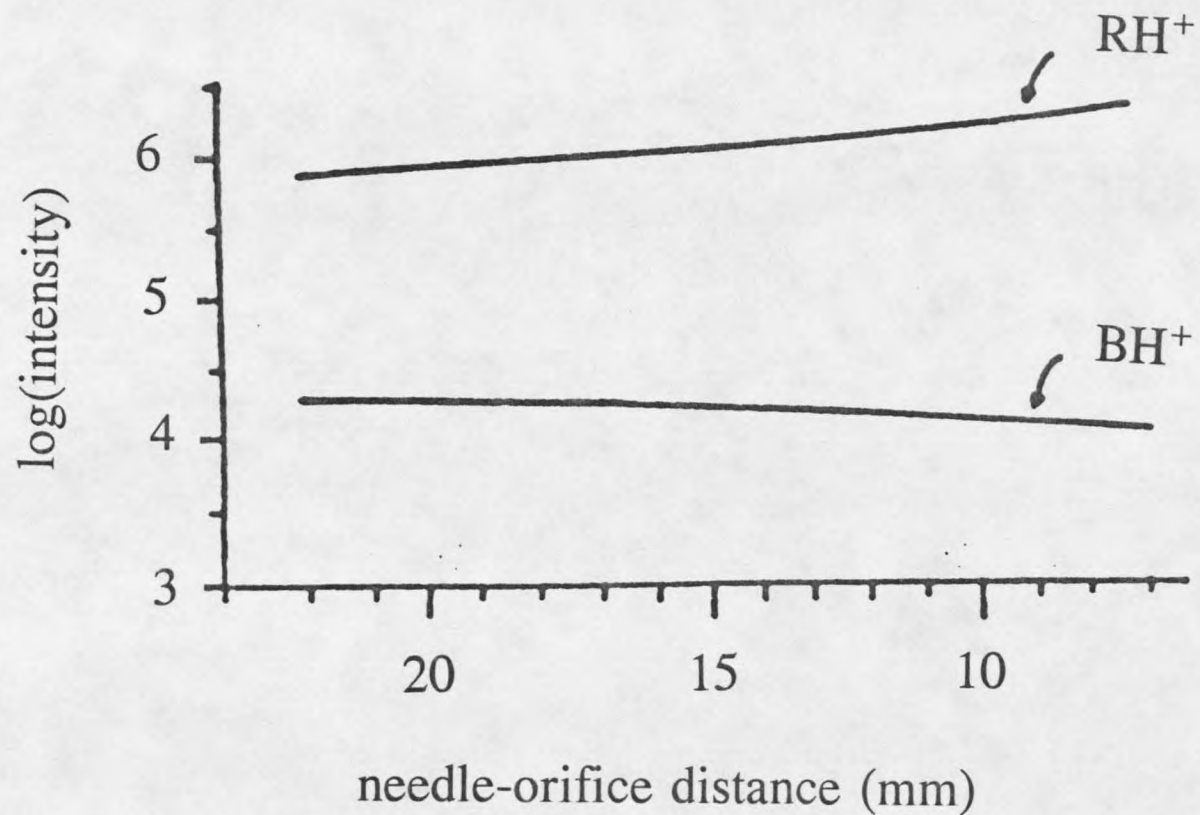


Figure 23. Calculated corona API ion currents: Based upon 0.1 ppb analyte (pyridine) concentration, 4mm of curtain gas and $\rho_0=10^{12}$ ions/cm³.

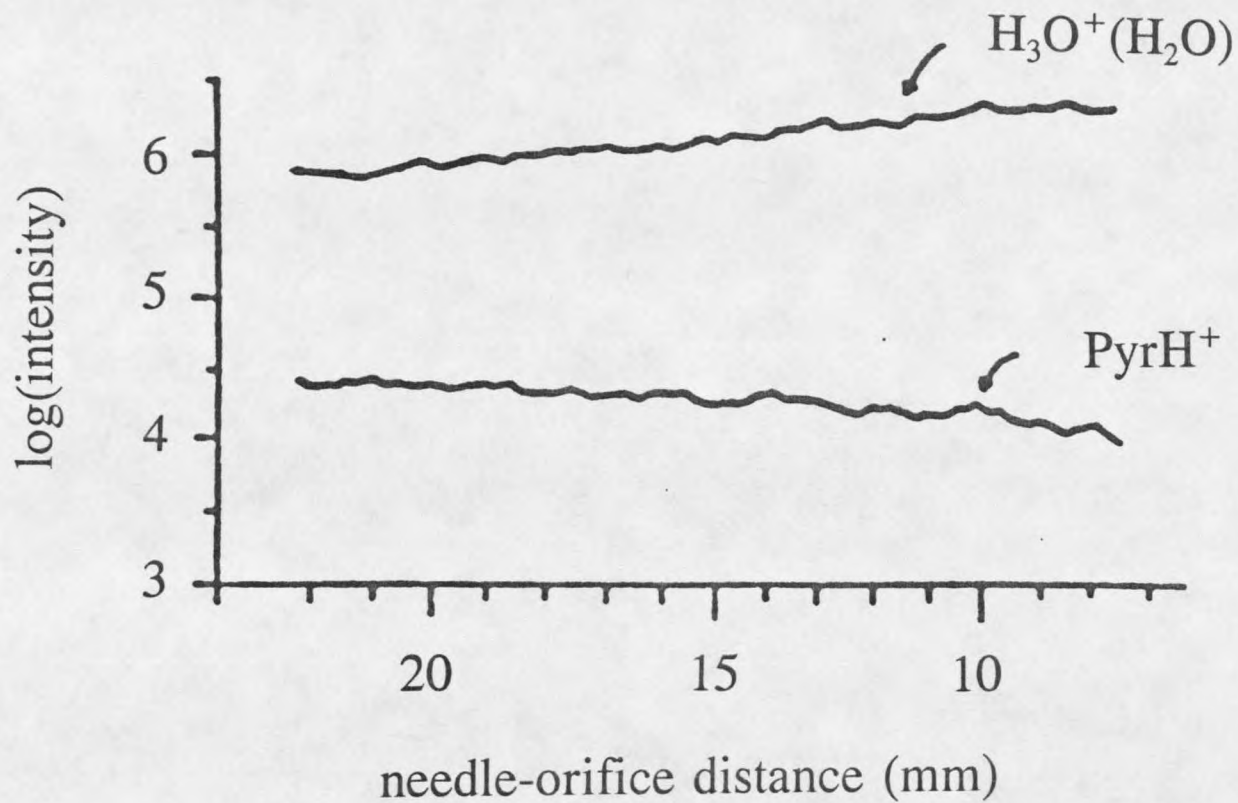


Figure 24. Experimental corona API ion currents: detailed in Reference (28).

equations into difference equations. It is the difference equations that are mapped over the grid. A variety of methods, including the finite difference and the finite element methods, have been developed to obtain a solution, based on the mapped difference equations. The obtained solution can be used to remap the difference equations on the grid. Typically, an iterative scheme is used to provide a "best" solution to the differential equations, based on the repeatedly remapped difference equations.²⁹

The rigorous numerical solution of a space charge system requires the use of such techniques. These methods require much computational time. The general concept of this application to space charge dominated systems has been discussed by Felici and Atten.^{17,30} Specific use of the technique to model space charge dominated systems has been made by Weber,³¹ McDonald,¹⁸ Leutert and Böhlen.³² Much of the work done in this area was done to model the operation of electrostatic precipitators. A good general work in this area, describing the space charge problems in electrostatic precipitators and how they relate to the general body of knowledge in electrostatics, has been written by Hinds.³³ In general, the work done to model precipitators involves geometries that are either cylindrical or planar. Work in the cylindrical geometries has been done mostly by using the analytical solution to the concentric cylindrical geometry. The planar geometry has required the use of finite

difference analysis of the parallel planar system. In the finite difference analysis, the geometry has been reduced to two dimensions by assuming the planar system to possess certain symmetry properties.³² Application of these numerical methods, to the modelling of space charge dominated mass spectrometry sources, has been made by Vogel.^{25,26}

Simulation Method

In addition to the actual numerical solving of the differential equations, another approach was used in the study of these systems. The previously discussed numerical methods for solving the differential equations, in addition to requiring large amounts of computer time, necessitate the stipulation of boundary conditions that are not available from the analysis of experimental conditions used for ion sources. An alternate simulation method was used to model these systems. In this method, the flow of ions is simulated by modelling the flow of ions through a grid of discrete cells.

The computer program written to allow a user to perform the simulation uses simple equations, previously described, to model the ion's movement as a response to the fields in the ion source. The coulombic forces between the source components and the drifting ions, as well as between the drifting ions and their own space charge field, are

considered. An initial field is set up, over the source, and an initial space charge in each of the source's discretized cells is assumed. Then, through a series of "time" steps, a current is introduced into the ion supply area of the source. The amount of charge introduced is appropriate to the length of the time step and the assumed current. As the simulation progresses, the conditions in each cell converge upon a steady state. For a source under simulation the steady state is assumed to give the desired information.

Simulation in General Geometries

With a simulation strategy in hand, attention can be turned to geometries out of the realm of the analytic solutions. These geometries include sources that are actually of more than one dimension. Interesting geometries that could be thought of as being mathematically two dimensional include the point to plane geometry and the finite length cylindrical geometry. These geometries are illustrated in Figures 25 and 26.

To discretize the source into a grid, the source must be divided so that the source is covered with a net of cells. The cells could be regular, such as a set of identically sized squares. However, one could attempt to concentrate the larger number of cells in the areas where the largest changes in the field conditions would be expected to occur. For the simulations, both approaches were

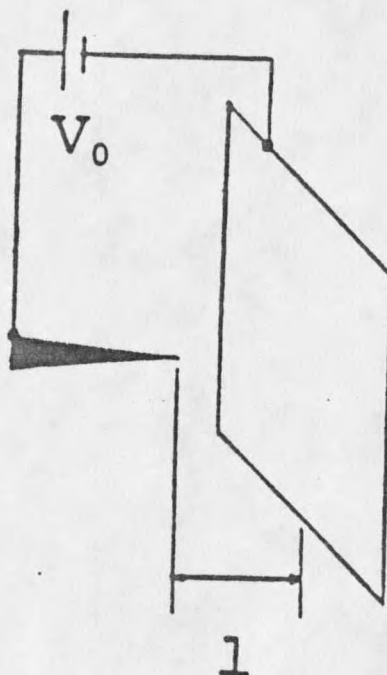


Figure 25. Point to plane geometry.

used. For some sources, with little need for a variable grid or little prior knowledge about source conditions, the grid was mapped with square or rectangular cells. Other sources, because of prior knowledge about the source conditions, were mapped with a parabolic grid. Figure 27 illustrates the geometry of the parabolic grid. The two dimensional grid, when rotated around the y-axis, forms a cylindrical geometry. Each cell then becomes a ring, centered around the y-axis. In this manner, the simulation gives the opportunity to model a variety of sources, providing that they possess

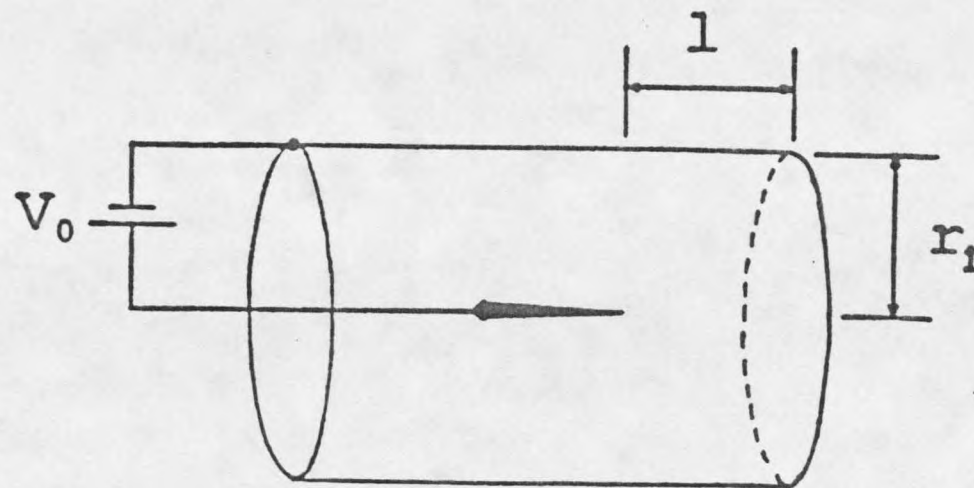


Figure 26. "Needle in can" geometry.

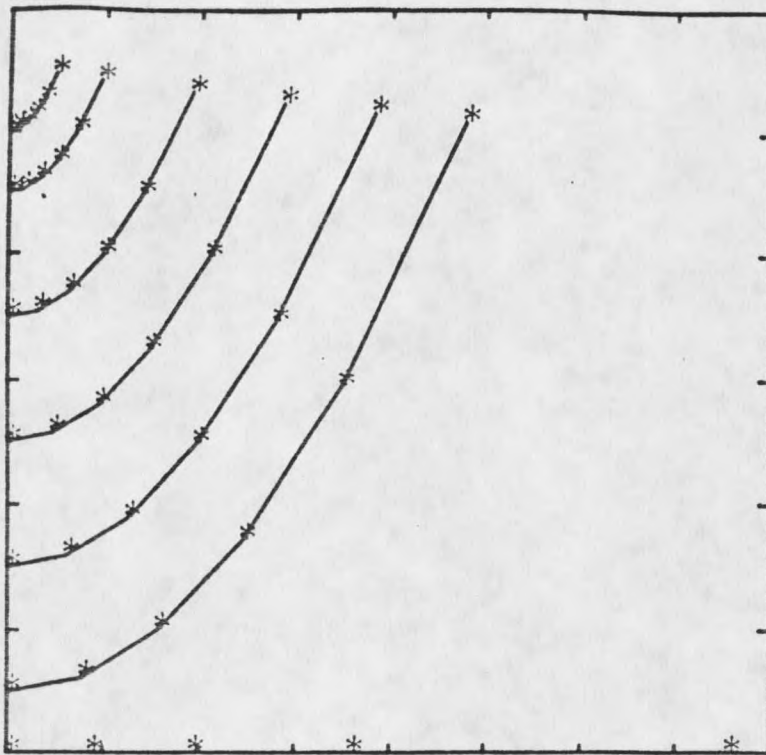


Figure 27. Parabolic grid.

symmetry around the axis of the cylindrical geometry. It is assumed that the axis of the geometry is perpendicular to the collector plate.

A separate mechanism for mapping an ion supply surface is needed for each geometry. The program user is given the opportunity to specify the current and details concerning the geometry of the supply surface. In the parabolic geometry, the user is asked to describe the width of the ion supply surface in terms of angular width. In the rectangular

grid geometry, the user is asked to describe a ring shaped supply surface by giving the rings inner and outer radii.

An intercellular distance is required for each cell to cell interaction. These distances are stored in an array. Based on the intercellular distances, fields can be calculated for each cell in the grid. These fields are a sum of both the Laplacian and space charge fields. The Laplacian fields result from fields calculated from a point charge that is placed at a specified distance behind the ion supply surface. The fields that each cell experiences are resolved into x- and y-components.

Upon the calculation of the fields for each cell, the program can allow for the movement of charge density throughout the grid. This movement is based on the components of the calculated ion velocities and the intercell distances. The fraction of the charge leaving a cell is based on a proportion of the distance travelled by ions in a cell to the size of the cell in which the ions are contained. A mechanism to allow for the movement of ions, based on space charge expansion in a single cell is provided.

The ion movement process also allows charge density to exit the entire grid, either by moving charge density to the collector plate or by hitting other defined source walls. The locations at which ion density exits the source are recorded.

The charge movement process repeats for a number of cycles. At the end of this set of cycles, the program recalculates the field strengths on the basis of the changed charge distribution. At certain intervals a charge grid and two field grids, describing, respectively, charge contained in each cell the x- and y- components of field strength in each cell, are saved by the computer. The progress of the simulation can be monitored by the examination of the calculated grids.

The "pseudo-time" intervals for charge movement, field recalculation and the total time of program operation are selected upon starting the simulation program. The times can be varied to be appropriate to the initial source parameters. Along with the time parameters, geometry type, needle charge and various source dimensions can be specified at the program's execution.

To enhance the applicability of the program, it was assumed that the collector plate would be constructed of a conducting material. A conductor, having a constant potential at every point, requires a special treatment for the calculation of electric fields. In this simulation the "method of mirrors." is used. This method places an imaginary mirror charge, on the other side of the conductor surface, for each charge. Therefore, each source component has a corresponding "mirror" component, and each grid cell has a corresponding "mirror" grid cell.

Point to Plane Geometry

For the point to plane geometry, the current intensity on the plate is of interest. Using the two dimensional simulation, a plot of current versus the distance from the axis of the geometry, was drawn. This plot is shown in Figure 28. This current distribution has previously been observed. An empirical modelling of this distribution has also been used by various workers.¹¹

Electrospray Geometry

In electrospray sources it has been noted that an interesting current distribution exists for a geometry that, at least at first glance, appears to look like a point to plane geometry. The current distribution is shown in Figure 29.²⁴ The contrast with the above modelled distribution is striking. This discrepancy can be explained by an important detail at the tip of the ESP needle. Instead of proceeding out of the needle in a straight jet, the liquid in the ESP can spread out in the form of droplets from the surface of a Taylor cone. However, often this Taylor cone is distorted into an umbrella shaped pattern. The droplets then seem to separate from the "rim" of the umbrella. The result is a ring shaped source of charged droplets, that are caused to drift towards the plate. The two forms of the electrospray flow are shown in Figures 30 and 31. The simulation of the "ring to plate" geometry gives an entirely different current

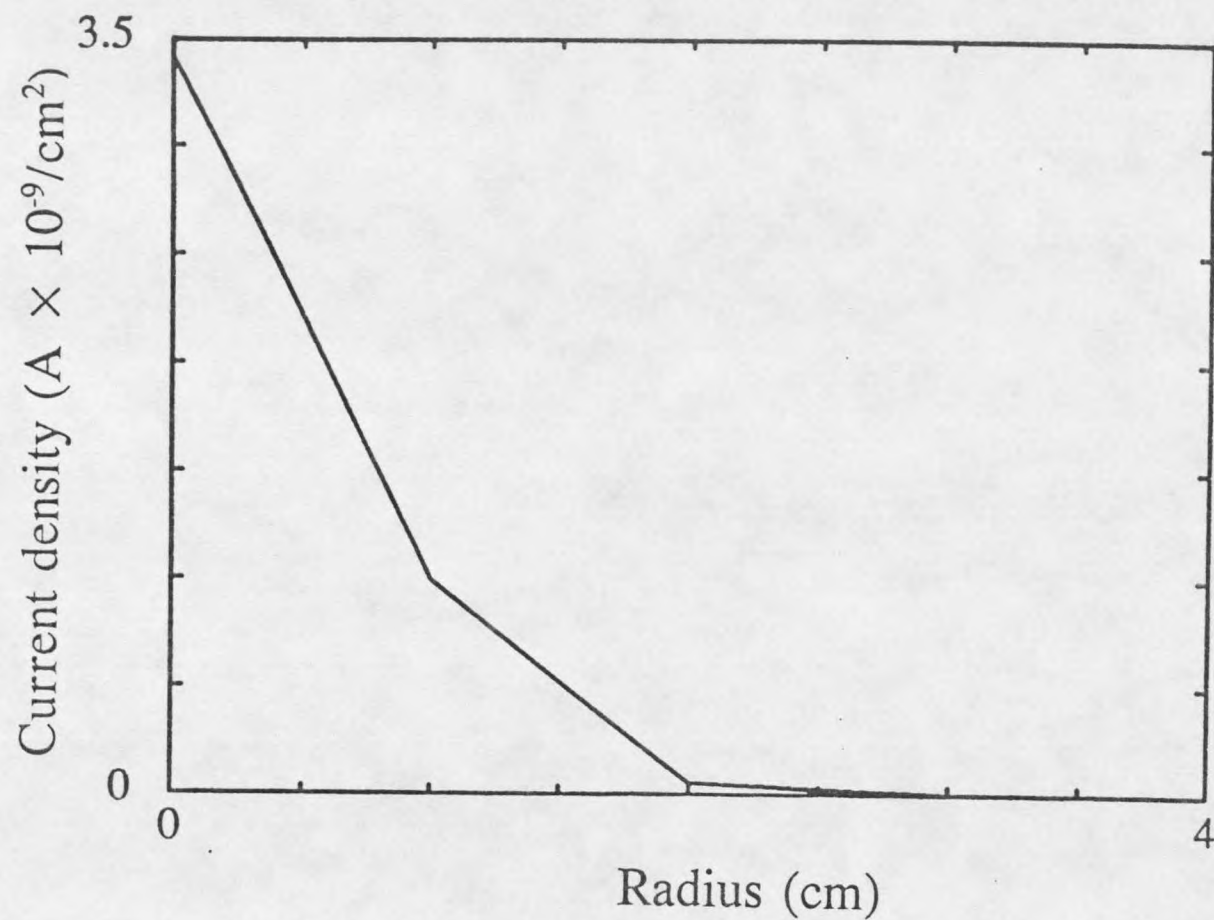


Figure 28. Calculated point to plane current distribution as a function of radius. For the calculation, the radius of the source is 4 cm, the length of the source is 5 cm, the current is 1×10^{-8} A, the needle charge is 1×10^{-6} C.

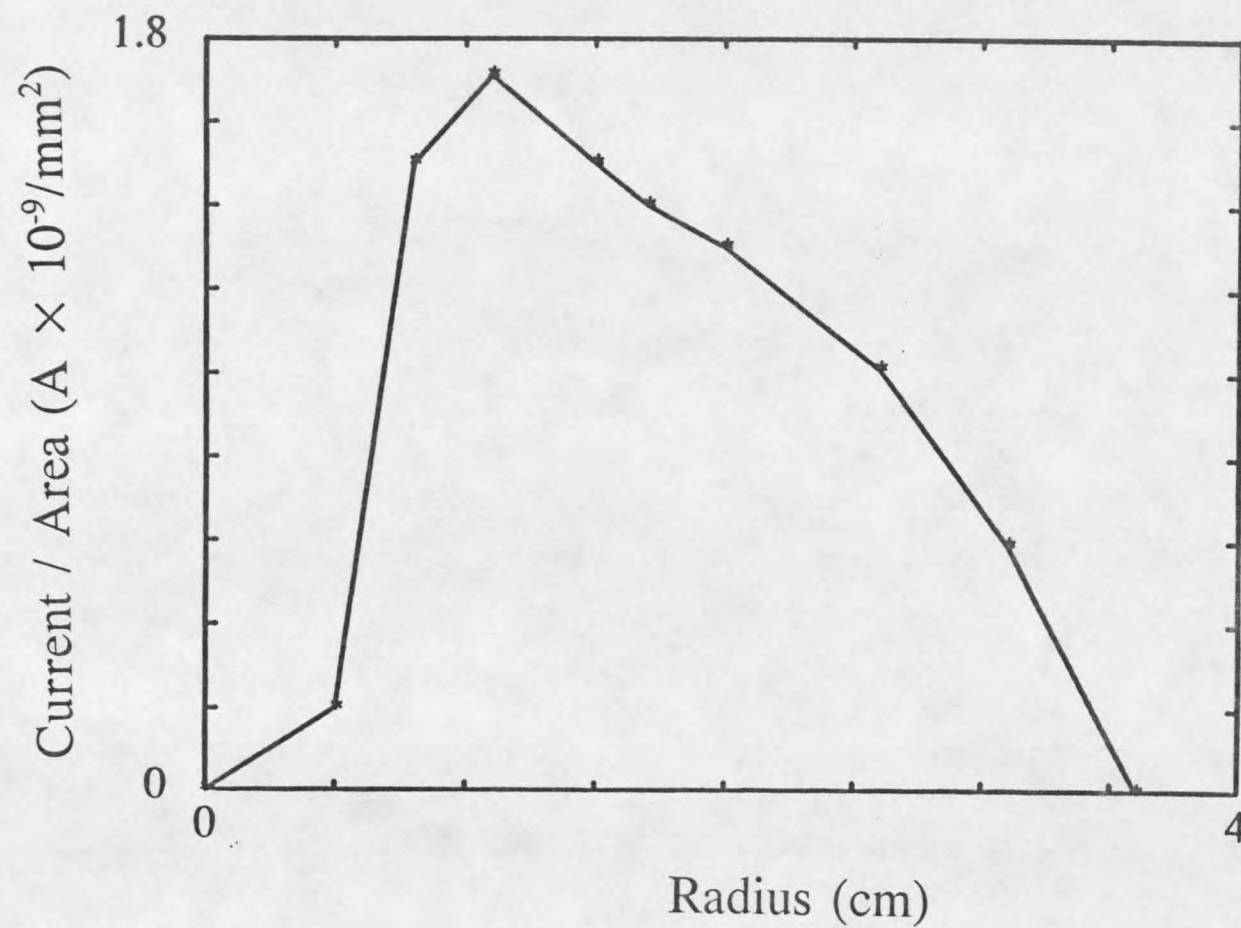


Figure 29. Experimental electrospray collector plate current distribution as a function of radius: detailed in Reference (25).

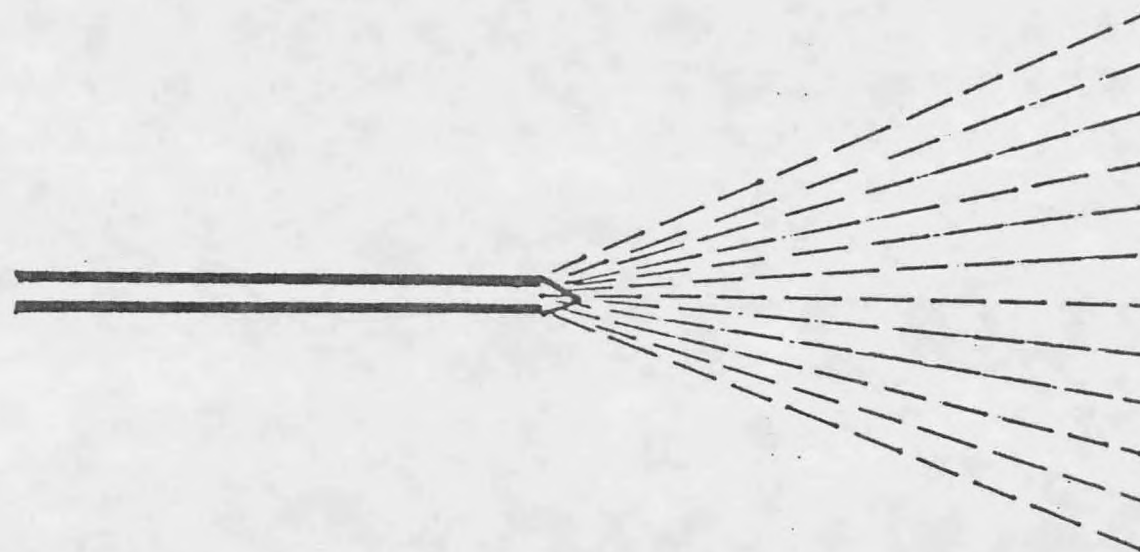


Figure 30. Spray pattern from a Taylor cone.

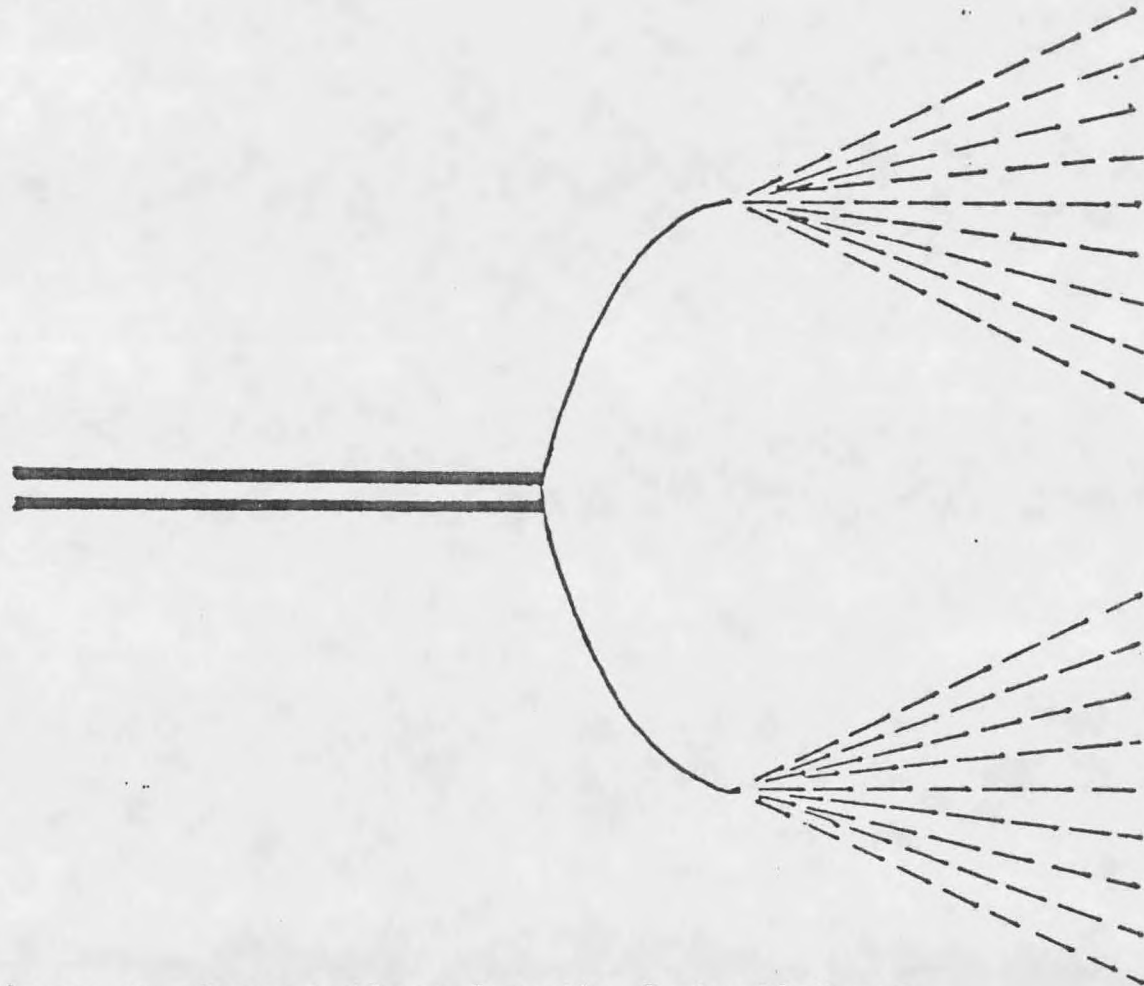


Figure 31. Spray pattern from the "umbrella" mode.

distribution. This distribution, shown in Figure 32, is seen to closely correspond to the experimentally observed distribution.

The contrast between the two current distributions is a direct consequence of the space charge effects, and cannot be explained in terms of Laplacian fields alone. The distribution can also be, at least qualitatively, described by using the unipolar space charge formula. The field and space charge density distributions for the electrospray source are shown in Figure 33.

API Geometry

Another interesting geometry, accessible with the two dimensional simulation, is the finite length cylindrical geometry. This geometry can be used to model the typical API source. This simulation is distinguished from the point to plane geometry by having defined walls, in addition to having a collector plate. Using standard operating parameters, a simulation can be used to model such things as current distributions on the source walls. Perhaps more importantly, it can be used to determine the degree of approximation that is made, when the spherical geometry, with its analytic solution, is used to model the API source. Results of the API simulation are shown in Figure 34 and 35.

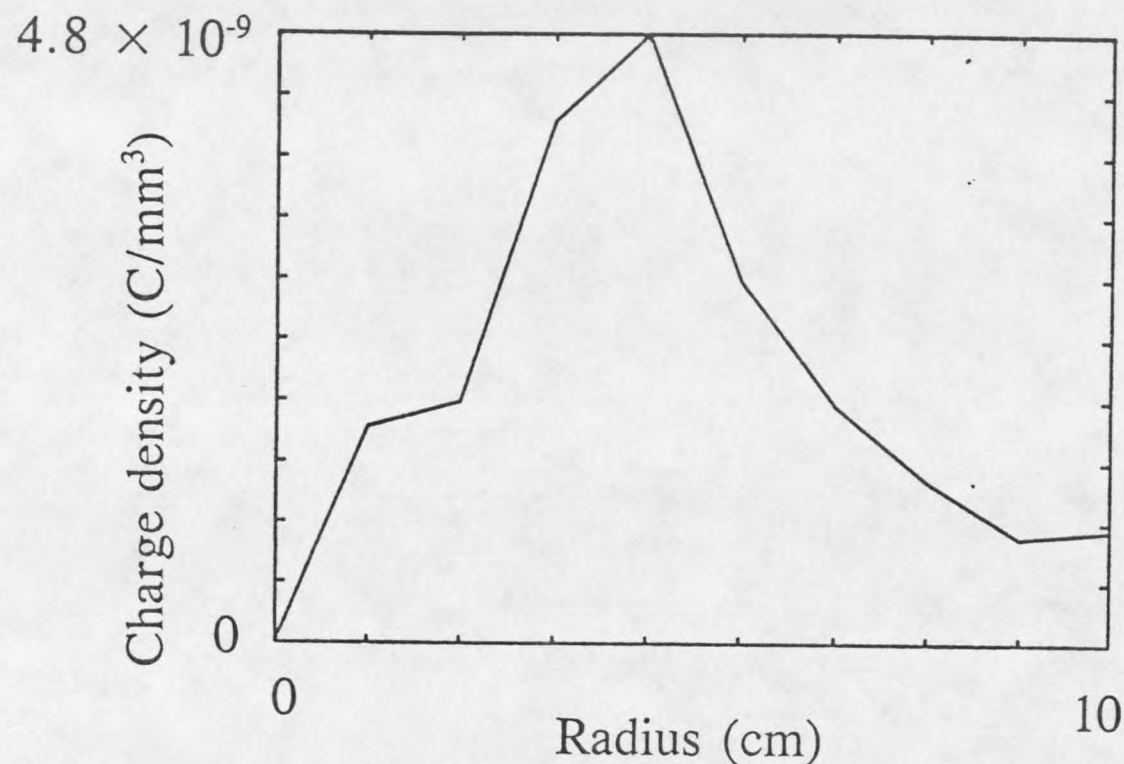


Figure 32. Calculated electro spray current distribution, at the collector plate, based upon ion densities at the perimeter of the source. For the calculation, the radius of the source is 10 cm, the length of the source is 2.5 cm, the electro spray current is 1×10^{-5} A, the electro spray needle charge is 1×10^{-6} C, and the electro spray current is injected into the source in a ring with inner and outer radii being 1.0 and 2.0 cm, respectively.

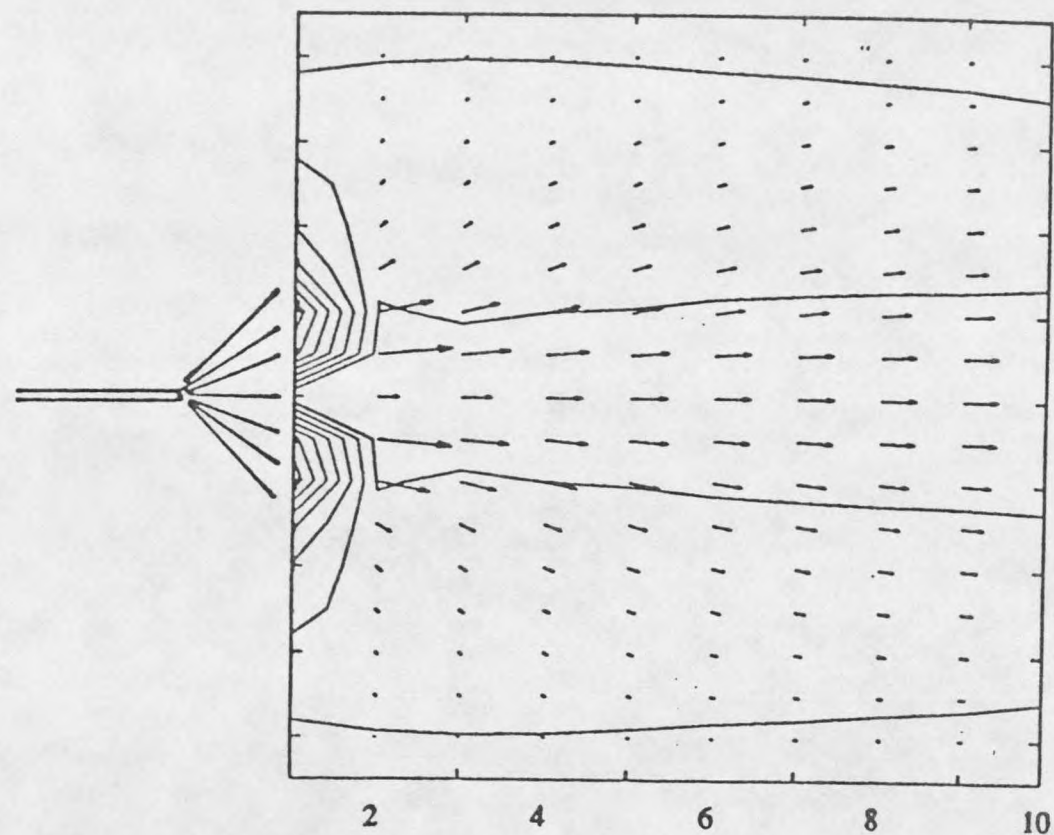


Figure 33. Field and space charge density contour for the electro spray simulation. The calculation parameters are the same as specified in Figure 32.

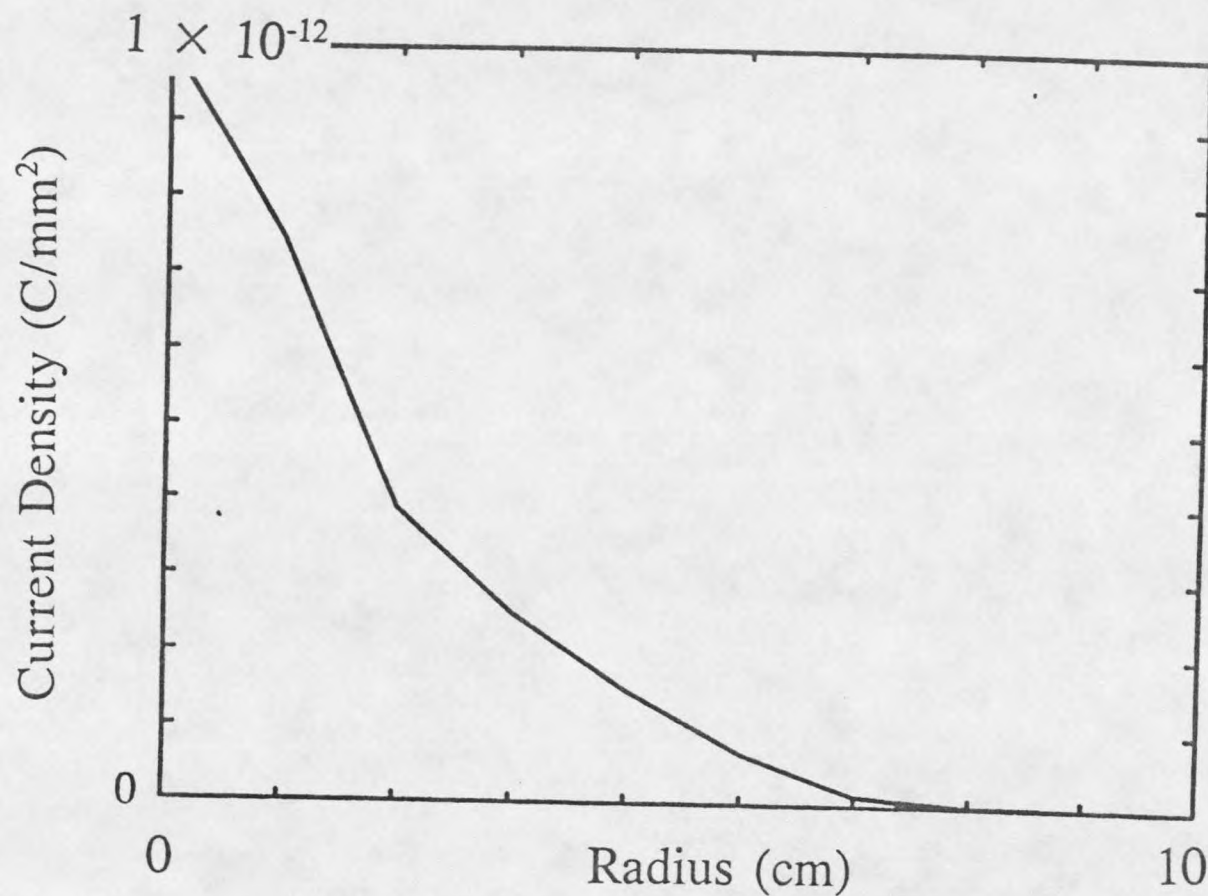


Figure 34. Calculated corona API current distribution at the collector plate. For the calculation, the radius of the source is 10 cm, the length of the source is 2.5 cm, the corona-API current is 1×10^{-9} A, the corona needle charge is 1×10^{-8} C, and the corona current is injected into the source in a circle with a radius of 2.0 cm.

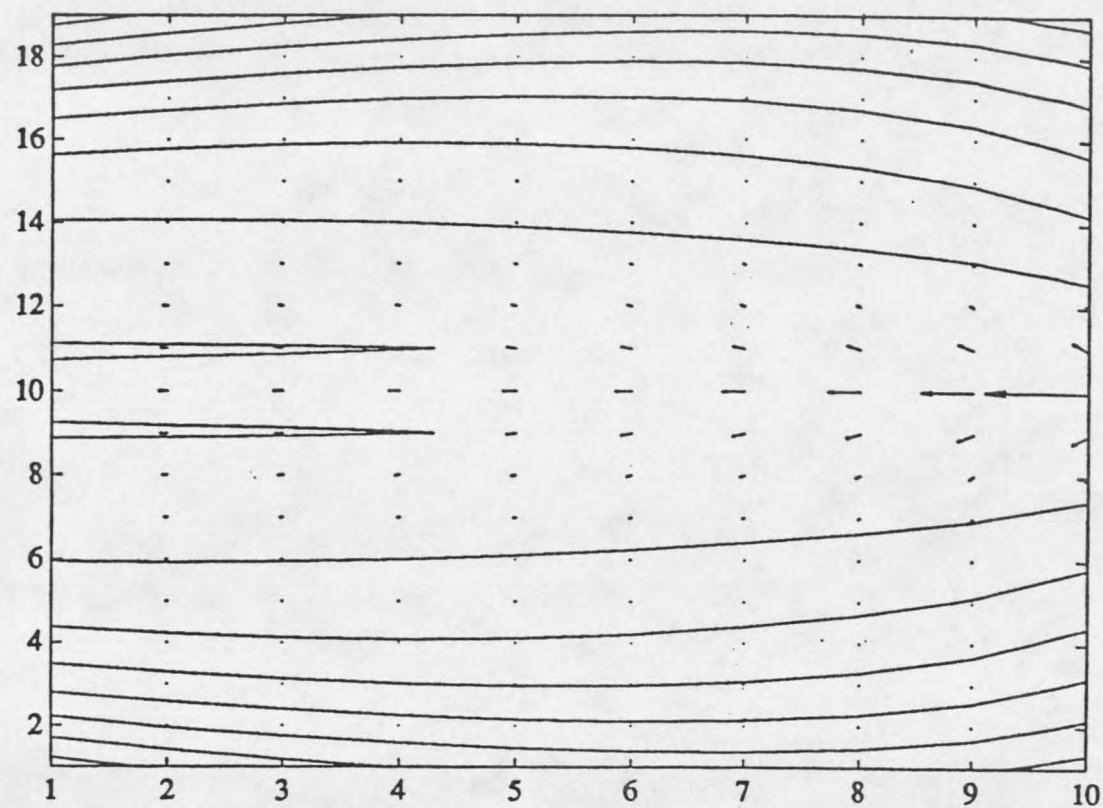


Figure 35. Field and space charge density contour for the corona API simulation. The calculation parameters are the same as specified in Figure 34.

TIME DEPENDENT CASE

The space charge model can be extended beyond steady state systems. The unipolar flow of ions in a dynamic system could be strongly influenced by space charge effects. An example of this type of system should demonstrate the utility of such an approach.

For this example, a cylindrical apparatus could be used. This cylinder would be constructed with conditions so that the Laplacian field strength would be constant throughout its entire length. This apparatus could be thought to represent, in a crude way, the ion tubes that are now used in many electrospray sources. The electrospray sources introduced by Fenn and Chait utilize ion tubes to transport ions from one region of the ion source to another. Figure 36 shows a schematic of such a source. A variety of materials have been successfully utilized for the ion tubes.^{7,34} Moreover, this apparatus can model drift tubes that are in use for ion mobility spectrometry (IMS).^{35,36}

To model ion transport in these ion tubes, it is convenient to imagine operating the system in pulse mode. To introduce ions into this system, ions would be filled behind a "gate" that would be a distance, a , from the source end of the tube. From the source plate to the gate, the ion

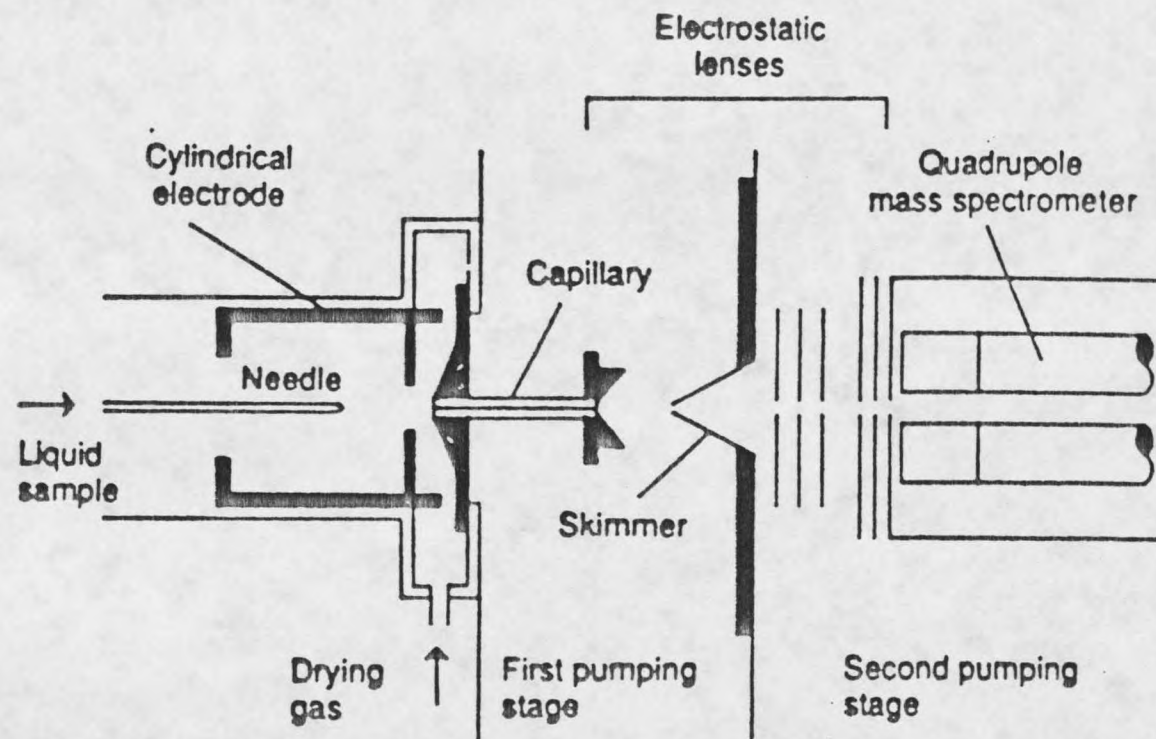



Figure 36. Ion tube in the Fenn electrospray source.

density, ρ_0 , would be constant. All ions in this region would be of the same mobility and charge. Between the gate and the collector plate, the ion density would be zero. The model system is illustrated in Figure 37.

At some time, t_0 , the gate would be 'opened' allowing the drift of the ions toward the collector plate. The velocity of the ion drift would be dependent on the field strength that each respective ion would experience. This field, as before, would be dependent on both the Laplacian field and the space charge field. Whether the space charge field would be important would depend on the initial space charge behind the gate.

Simulation With One Type of Ion

The ion tube is treated here by using the infinite parallel plate geometry. This treatment is based on the assumption that both systems have constant Laplacian field strength throughout their entire lengths. A computer model of this system was constructed. In this model, the length of the drift tube was divided into cells of equal length. The number of cells could be chosen on the basis of the desired accuracy of the model. The cells were each filled with ion density appropriate to the initial conditions. At the each end of the tube was a plate of a certain assigned charge. The model then went through a series of time steps. At each time step the actual field strength in each cell was

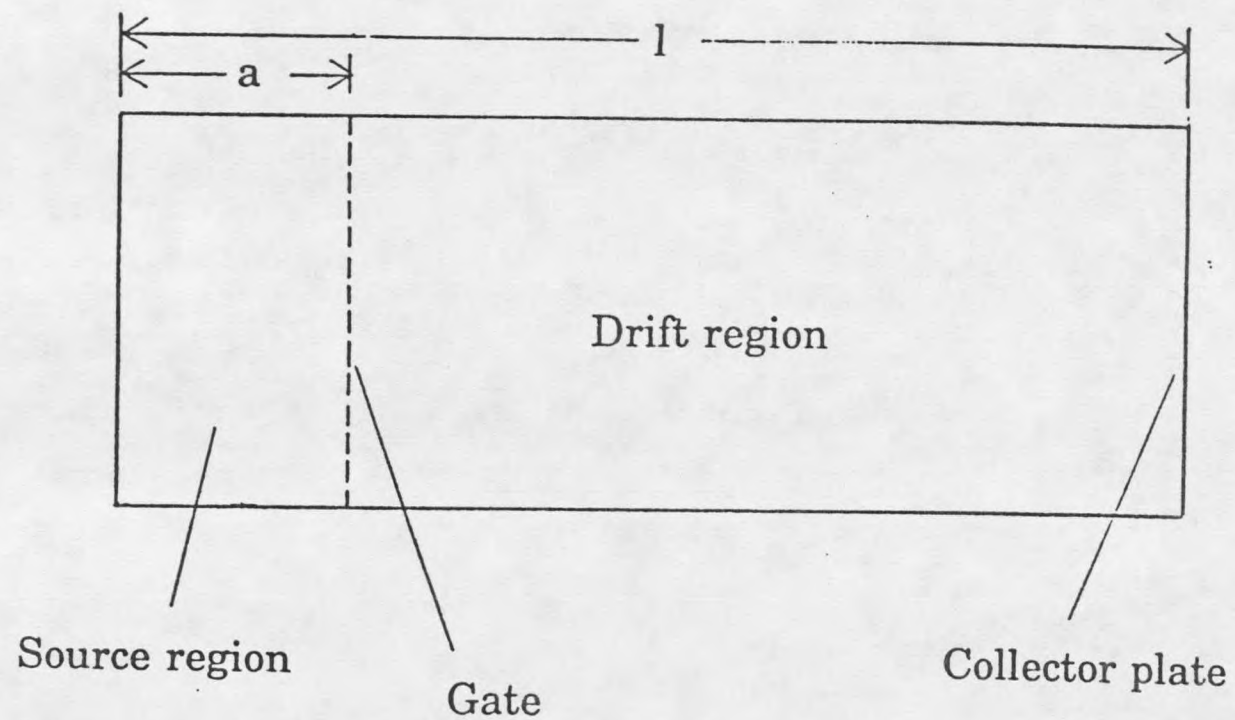

75

Figure 37. Drift tube schematic.

calculated. This field strength, in turn, gave a drift velocity for the ions in each cell. The length of the timestep multiplied by the length of the timestep would give an indication of the displacement of ion density out of each cell. At the end of each timestep, a new ion density distribution, appropriate to the ion displacements, was constructed. To record the simulation of the ion flow, the ion collection current, at the collector plate, was recorded as a function of time. This collection current is shown in Figure 38.

Simulation With Two Types of Ions

As a further example of the utility of this approach, a similar program was written to allow the presence of two types of ions in the tube. The construction of the model was the same as in the preceding example, except for the need to account for two separate ion densities in each cell. The two ion types were assumed to have different ion mobilities. For the simulation, one ion type, ion A, was given an ionic mobility, $\kappa_A = 4 \text{ m}^2/\text{V}\cdot\text{s}$. The second ion type, ion B, was given an ion mobility, $\kappa_B = 2 \text{ m}^2/\text{V}\cdot\text{s}$.

The collection current for this simulation is shown in Figure 39. The current profile, as a function of time, displays the modification of chromatography, based on ionic mobilities, by space charge. This chromatography, ion mobility spectrometry (IMS), is based on transport in the

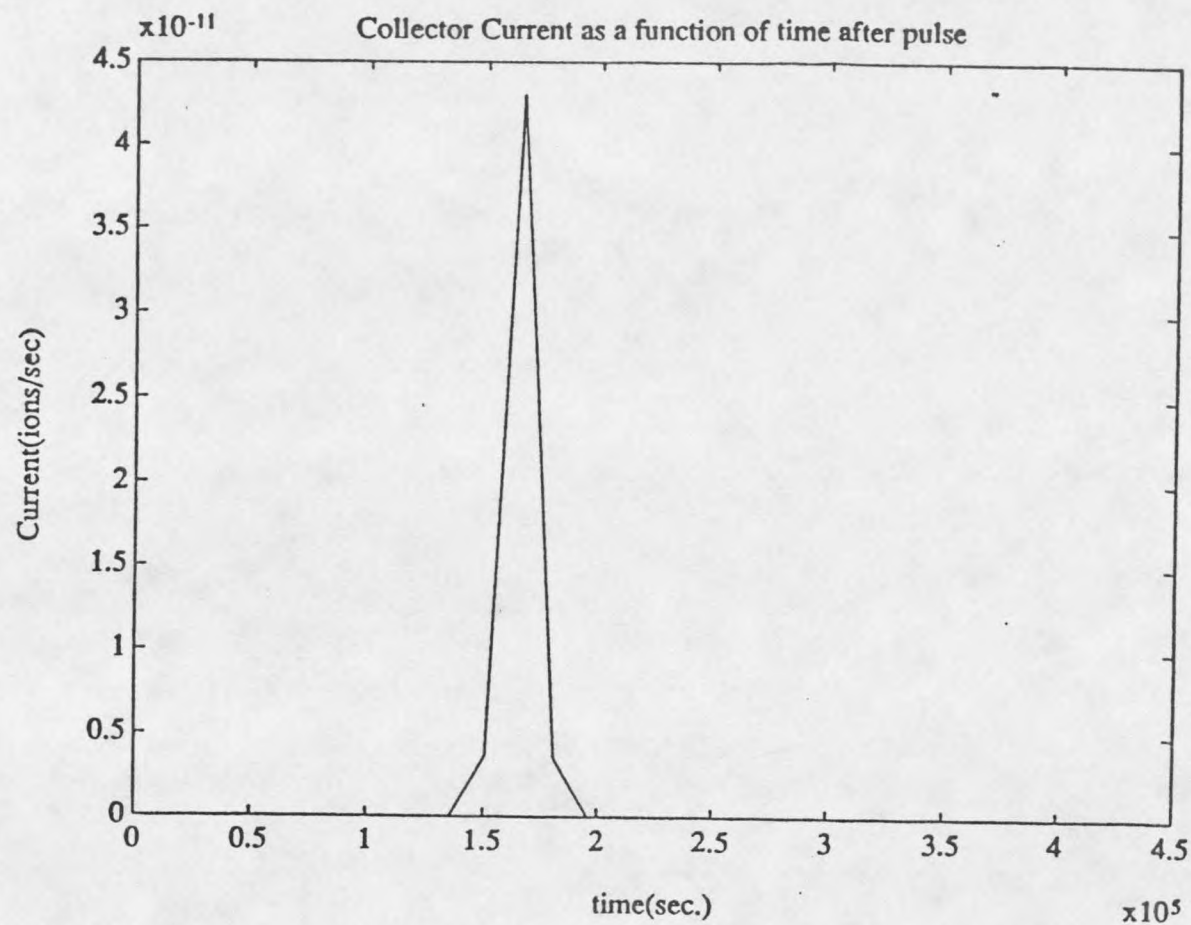


Figure 38. One component ion drift current versus time. The ion mobility for the drifting ion is $2 \times 10^{-4} \text{ m}^2/\text{V}\cdot\text{s}$. The field strength in the drift region is 0.5 V/m . The pulse contains 5×10^{-7} ions.

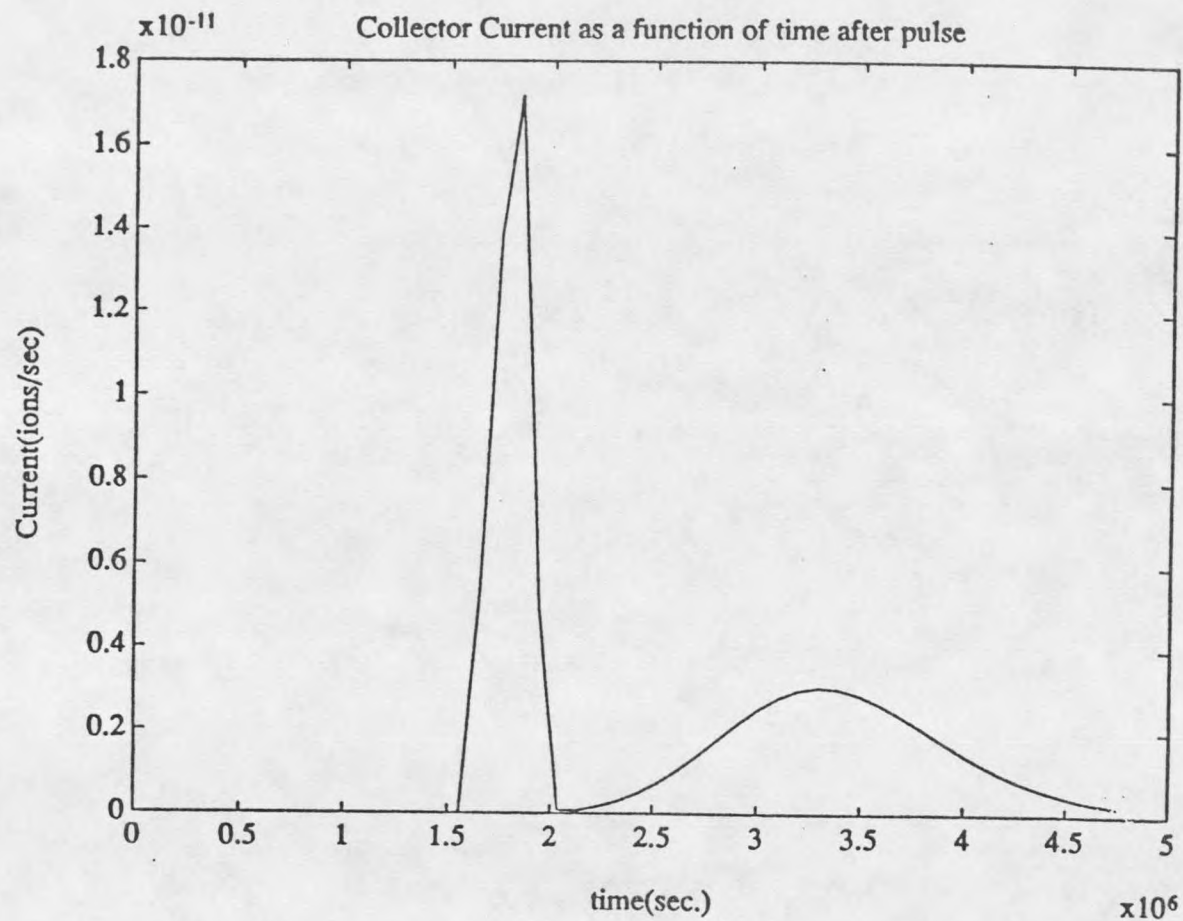


Figure 39. Two component ion drift current versus time. The field strength in the drift region is 0.05 V/m. The pulse contains 5×10^{-6} ions of each drifting species.

ion tube being a function of ion mobility.³⁴

In the case of the ion tube in the electrospray source, the actual retarding effects in the ion flow are not well understood. The importance, in the ion transport, of adsorption of the ions on the ion tubes walls, the degree of hydration of the ions and fluid flow considerations are not well understood and are presently the subject of experimental study. Furthermore, in typical uses of these ion tubes, the effect of the ion transport through the tube may often be overwhelmed by the events occurring at both the entrance and the exit to the tube. The fluid and coulombic influences on ion flow would seem to be difficult to monitor, or model, in these regions. Clearly, additional work will be necessary in this area.

SUMMARY

In this work, ion transport in unipolar mass spectrometry ion sources like corona API and electrospray has been studied theoretically. Unlike previous work in this area, the study has been done with the consideration of space charge effects. Analytic solutions of the space charge problem have been obtained for simple ion geometries, including the cases of infinite parallel planes, concentric cylinders of infinite length, and concentric spheres. These analytic solutions allow, for their respective geometries, the calculation of electric field, potential, ion density distributions, and ion residence times. It is shown that for typical operating conditions, the minimum potential required to overcome the space charge effect in corona API, or electrospray ion sources, constitutes a dominant or significant fraction of the total applied voltage. Further, the electric field, in the region of the ion sampling orifice and the ion residence time in the ion source are determined mainly by the space charge. Extending the approach to more general geometries, use of the unipolar formula, numerical methods of differential equations and a simulation approach was made. With the unipolar formula, absolute sensitivities of corona API ion sources were

calculated. Also, general geometries were modelled by a simulation calculation. The calculation was based on a computer program written to model ion flow in various ion sources having different geometries. Finally, the space charge influenced ion drift in a drift tube-type apparatus was modelled, as a function of time.

The analyses, for the first time, provide methods for evaluating the ion sampling efficiency in high pressure, high current ion sources such as corona API and electrospray. Also, presented for the first time is a method for evaluating absolute sensitivities in the corona API source.

REFERENCES CITED

1. Dempster, W., "A New Method of Positive Ray Analysis," Phys. Rev., 11, 1918, 316-325.
2. Bleakney, W. "A New Method of Positive Ray Analysis and its Application to the Measurement of Ionization Potentials in Mercury Vapor," Phys. Rev., 34, 1929, 157-160.
3. Munson, M.S.B., Field, F.H., "Chemical Ionization Mass Spectrometry," J. Am. Chem. Soc., 88, 1966, 2621-2630.
4. Barber, M.N., Bordoli, R.S., Sedgick, R.D., Tyler, A.N., "Fast Atom Bombardment of Solids (F.A.B.): A New Ion Source for Mass Spectrometry," J. Chem. Soc., Chem. Commun., 7, 1981, 325-327.
5. Mitchum, R.K., Korfmacher, W.A., "Atmospheric Pressure Ionization Mass Spectrometry," Anal. Chem., 55, 1983, 1485A-1496A.
6. Vestal, M.L., "Studies of Ionization Mechanisms Involved in Thermospray LC-MS," J. Mass Spectrom., 46, 1983, 193-196.
7. Fenn, J.B., Mann, M., Meng, C.K., Wong, S.F., Whitehouse, C.M., "Electrospray Ionization for Mass Spectrometry of Large Biomolecules," Science, 246, 1989, 64-71.
8. Chapman, S., "Carrier Mobility Spectra of Spray Electrified Liquids," Phys. Rev., 52, 1939, 184-190.
9. Chapman, S., "The Magnitude of the Corona Point Discharge Current," Journal of Atmospheric Sciences, 34, 1977, 1801-1809.
10. Loeb, L.B. Basic Processes of Gaseous Electronics, University of California Press, Berkeley, 1955.
11. Sigmond, R.S., "Electrical Coronas," Electrical Breakdown of Gases, Meek, J.M. and Craggs, J.D. (ed.) Wiley, New York, 1978.
12. Townsend, J.S., "The Potentials Required to Maintain Currents Between Coaxial Cylinders," Phil. Mag., 28, 1914, 83-90.
13. McDaniel, E.W., Mason, E.A., The Mobility and Diffusion of Ions in Gases, John Wiley and Sons, New York, 1973.
14. Abou-Seada, M.S., Nasser, E., "Digital Computer Calculation of the Electric Potential and Field of a Rod Gap," Proceedings of the IEEE, 56, 1968, 813-820.

15. Child, C.D., "Discharge from Hot CaO," Phys. Rev., 32, 1908, 492-511.
16. Langmuir, I., "The Effect of Space Charge and Residual Gases on Thermionic Currents in High Vacuum," Phys. Rev., 2, 1913, 450-486.
17. Felici, N., "Recent Advances in the Analysis of D.C. Ionised Electric Fields," Dir. Curr., 8, 1963, 252-260, 278-287.
18. McDonald, J.R., Smith, W.B., Spencer, H.W., Sparks, L.E., "A Mathematical Model for Calculating Electrical Conditions in Wire-Duct Precipitation Devices," J. Appl. Phys., 48, 1977, 2231-2243.
19. Shahin, M.M., "Mass-Spectrometric Studies of Corona Discharges in Air at Atmospheric Pressures." J. Chem. Phys., 45, 1966, 2600-2605.
20. Gobby, P.L., Grimsrud, E.P., Warden, S.W., "Improved Model of the Pulsed Electron Capture Detector," Anal. Chem., 52, 1980, 473-482.
21. Chapman, S., Discharge of Corona Current from Points on Aircraft or on the Ground, Cornell Aeronautical Laboratory, Buffalo, 1955.
22. Chapman, S., Corona Discharge from an Isolated Point in Wind, Rep. No. 161, Cornell Aeronautical Laboratory, Buffalo, 1967.
23. Rees, J.A., "Fundamental Processes in the Electrical Breakdown of Gases," Electrical Breakdown of Gases, Meek, J.M. and Craggs, J.D. (ed.), Wiley, New York, 1978.
24. Iribarne, J.B., Thomson, B.A., "On the Evaporation of Small Ions from Charged Droplets," J. Chem. Phys., 64, 1976, 2287-2294.
25. Ikonomou, M.G., Blades, A.T., Kebarle, P., "Investigations of the Electrospray Interface for Liquid Chromatography/Mass Spectrometry," Anal. Chem., 62, 1990, 957-967.
26. Vogel, C., Busman, M., Sunner, J., in preparation.
27. Busman, M., Sunner, J., Vogel, C., "Space-Charge Dominated Mass Spectrometry Ion Sources: Modelling and Sensitivity," J. Am. Soc. Mass Spectrom., 2, 1991, 1-10.

28. Sunner, J., Nicol, G., Kebarle, P., "Factors Determining the Relative Sensitivity of Analytes in Positive Mode Atmospheric Pressure Ionization Mass Spectrometry," Anal. Chem., 60, 1988, 1300-1307.
29. Botha, J.F., Pinder, G.F., Fundamental Concepts in the Numerical Solution of Differential Equations, Wiley-Interscience, New York, 1983.
30. Atten, P., "Methode Generale de Resolution du Probleme du Champ Electrique Modifie par Une Charge D'Espace Unipolaire Injectee." Rev. Gen. de Electr., 83, 1974, 143-153.
31. Weber, C., "Numerical Solution of Laplace's and Poisson's Equations and the Calculation of Electron Trajectories and Electron Beams," Chapter 1.2, Focusing of Charged Particles, Vol. 1, Septier, A. (ed.), Academic Press, New York, 1967.
32. Leutert, G., Bohlen, B., "Der Raumliche Verlauf von Elektrischer Feldstarke und Raumladungsdichte im Platten-Elektrodefilter," Staub, 32, 1972, 297-301.
33. Hinds, W.C., Aerosol Technology. Properties, Behavior, and Measurement of Airborne Particles, John Wiley and Sons, New York, 1982.
34. Chowdhury, S.K., Katta, V., Chait, B.T., "An Electrospray Ionization MS with New Features for Protein Analysis," Presented at the 38th ASMS Conference on Mass Spectrometry and Allied Topics, June 3-8, 1990.
35. Revercomb, H.E., Mason, E.A., "Theory of Plasma Chromatography / Gaseous Electrophoresis - A Review," Anal. Chem., 47, 1975, 970-983.
36. Cohen, M.J., Karasek, F.W., "Plasma Chromatography-A New Dimension for Gas Chromatography and Mass Spectrometry," J. Chromatogr. Sci., 8, 1970, 330-337.

APPENDICES

APPENDIX A
ANALYTIC SOLUTIONS

Derivations of field strength expressions for planar, cylindrical and spherical geometries are shown.

Planar geometry

The ion current density, J , is

$$J = \rho \cdot v, \quad (35)$$

where v is the ion density. Also,

$$i = J \cdot A, \quad (36)$$

where i is the ion current and A is the unit area. So,

$$i = J. \quad (37)$$

The ion velocity, v , is

$$v = K \cdot E. \quad (38)$$

The space charge density, ρ , becomes

$$\rho = \frac{J}{v} = \frac{i}{K \cdot E}. \quad (39)$$

The Poisson equation in the planar geometry is

$$\nabla^2 V = \frac{\rho}{\epsilon_0} \quad (40)$$

$$= \frac{d}{dx} \left[\frac{dV}{dx} \right] \quad (41)$$

$$= \frac{dE}{dx}. \quad (42)$$

This equation, with the expression for space charge, ρ_0 , can be integrated to give E.

$$dE = \frac{\rho}{\epsilon_0} dx = \frac{i}{\epsilon_0 K E} dx \quad (43)$$

$$\int_{E_0}^E dE = \frac{i}{\epsilon_0 K} \int_0^x dx \quad (44)$$

$$E = \left(\frac{2i}{\epsilon_0 K} x + E_0^2 \right)^{1/2} \quad (45)$$

$$E^2 = \frac{2i}{\epsilon_0 K} x + E_0^2 \quad (46)$$

Using the relation

$$\rho = \frac{i}{K \cdot E}, \quad (47)$$

the space charge density is given by

$$\rho = \frac{i}{K} \left[\frac{2i}{\epsilon_0 K} x + E_0^2 \right]^{1/2}. \quad (48)$$

Cylindrical Geometry

The ion current density, J , is

$$J = \rho \cdot v \quad (49)$$

and the ion current, i , is

$$i = J \cdot A, \quad (50)$$

where A is the surface area of a unit length of the cylinder, with a radius, r . The surface area, A , is given by

$$A = 2\pi r. \quad (51)$$

Using,

$$v = K \cdot E \quad (52)$$

for ion velocity, the space charge density, ρ , becomes

$$\rho = \frac{i}{2\pi r K E}. \quad (53)$$

The Poisson equation for a cylindrically symmetric geometry is

$$\nabla^2 V = \frac{\rho}{\epsilon_0} \quad (54)$$

$$= \frac{1}{r} \frac{d}{dr} \left[r \frac{dV}{dr} \right] \quad (55)$$

$$= \frac{1}{r} \frac{d}{dr} (rE) . \quad (56)$$

Using the above expression for space charge density, ρ , one obtains

$$\frac{1}{r} \frac{d}{dr} (rE) = \frac{i}{2\pi r K E \epsilon_0} , \quad (57)$$

or upon rearrangement

$$(rE) \frac{d}{dr} (rE) = \frac{ri}{2\pi r K E \epsilon_0} . \quad (58)$$

This equation can be integrated to give an expression for field strength, E .

$$\int_{r_0 E_0}^{rE} (rE) d(rE) = \frac{i}{2\pi K \epsilon_0} \int_{r_0}^r r dr \quad (59)$$

$$(rE)^2 \Big|_{r_0 E_0}^{rE} = \frac{i}{2\pi K \epsilon_0} r^2 \Big|_{r_0}^r \quad (60)$$

$$r^2 E^2 - r_0^2 E_0^2 = \frac{i}{2\pi K \epsilon_0} (r^2 - r_0^2) \quad (61)$$

$$r^2 E^2 = \frac{i}{2\pi K \epsilon_0} (r^2 - r_0^2) + r_0^2 E_0^2 \quad (62)$$

$$E^2 = \frac{r_0^2}{r^2} \left[\frac{i}{2\pi K \epsilon_0} \frac{r^2}{r_0^2} - \frac{i}{2\pi K \epsilon_0} + E_0^2 \right] \quad (63)$$

$$E = \frac{r_0}{r} \left[\frac{i}{2\pi K \epsilon_0 r_0^2} (r^2 - r_0^2) + E_0^2 \right]^{1/2} \quad (64)$$

Using the relation

$$\rho = \frac{i}{2\pi r K E}, \quad (65)$$

the space charge density is then given by

$$\rho = \frac{i}{2\pi r_0 K} \left[\frac{i}{2\pi K \epsilon_0 r_0^2} (r^2 - r_0^2) + E_0^2 \right]^{-1/2}. \quad (66)$$

Spherical geometry

The ion current density, J , is

$$J = \rho \cdot v, \quad (67)$$

and the ion current, i , is

$$i = J \cdot A, \quad (68)$$

where the area, A , is the surface area of a sphere of radius, r ,

$$A = 4\pi r^2 \quad (69)$$

The ion velocity, v , is

$$v = K \cdot E. \quad (70)$$

The space charge density, ρ , can then be given as

$$\rho = \frac{i}{4\pi r^2 K E}. \quad (71)$$

The Poisson equation for a spherically symmetric geometry is

$$\nabla^2 V = \frac{\rho}{\epsilon_0} \quad (72)$$

$$= \frac{1}{r^2} \frac{d}{dr} \left[r^2 \frac{dV}{dr} \right] \quad (73)$$

$$= \frac{1}{r^2} \frac{d}{dr} (r^2 E). \quad (74)$$

With the use of the above expression for space charge density, ρ , one obtains

$$\frac{1}{r^2} \frac{d}{dr} (r^2 E) = \frac{i}{4\pi \epsilon_0 K E r^2}. \quad (75)$$

This equation can be integrated to give an expression for E .

$$d(r^2 E) = \frac{i}{4\pi \epsilon_0 K E} dr \quad (76)$$

$$(r^2 E) \, d(r^2 E) = \frac{i}{4\pi\epsilon_0 K} r^2 dr \quad (77)$$

$$\int_{r_0^2 E_0}^{r^2 E} (r^2 E) \, d(r^2 E) = \frac{i}{4\pi\epsilon_0 K} \int_{r_0}^r r^2 dr \quad (78)$$

$$\frac{1}{2} (r^2 E)^2 \Big|_{r_0^2 E_0}^{r^2 E} = \frac{i}{4\pi\epsilon_0 K} \frac{1}{3} r^3 \Big|_{r_0}^r \quad (79)$$

$$r^4 E^2 - r_0^4 E_0^2 = \frac{i}{6\pi\epsilon_0 K} (r^3 - r_0^3) \quad (80)$$

$$r^4 E^2 = \frac{i}{6\pi\epsilon_0 K} (r^3 - r_0^3) + r_0^4 E_0^2 \quad (81)$$

$$E^2 = \left(\frac{r_0}{r} \right)^4 E_0^2 + \frac{i}{6\pi\epsilon_0 K} \left(\frac{r^3}{r^4} - \frac{r_0^3}{r^4} \right) \quad (82)$$

$$E = \left(\frac{r_0}{r} \right)^2 \left[\frac{i}{6\pi\epsilon_0 K r_0^4} (r^3 - r_0^3) + E_0^2 \right]^{1/2} \quad (83)$$

Then using

$$\rho = \frac{i}{4\pi r^2 K E}, \quad (84)$$

the space charge density can be given as

$$\rho = \frac{i}{4\pi\epsilon_0 r_0^2 K} \left[\frac{i}{6\pi\epsilon_0 K r_0^4} (r^3 - r_0^3) + E_0^2 \right]^{-1/2}. \quad (85)$$

APPENDIX B
DERIVATIONS FOR LIMITING CONDITIONS.

Derivations of expressions for ion residence time, t_{res} , sampling ion density, ρ_{samp} , and applied potential, V_0 , at the limit of space charge domination and $r_0 \ll r$ in a spherically symmetric system are shown.

Ion residence time, t_{res}

The expression for field strength, E , in spherical geometry is

$$E = \left(\frac{r_0}{r} \right)^2 \left[E_0^2 + \frac{i}{6\pi\epsilon_0 K} \left(\frac{r^3}{r_0^4} - \frac{r_0^3}{r^4} \right) \right]^{1/2}. \quad (86)$$

Upon application of the limit $E_0 > 0$,

$$E = \left(\frac{i}{6\pi\epsilon_0 K} \left(\frac{1}{r} - \frac{r_0^3}{r^4} \right) \right)^{1/2}. \quad (87)$$

Now, if $r_0 \ll r$, the field strength, E , becomes

$$E = \left(\frac{i}{6\pi\epsilon_0 K} \frac{1}{r} \right)^{1/2} \quad (88)$$

The velocity, v , of ions in the source is given by the drift equation,

$$v = K \cdot E = \frac{dr}{dt}. \quad (89)$$

Substituting the above relation for E , into the drift equation gives

$$\frac{dr}{dt} = K \left[\frac{i}{6\pi\epsilon_0 K r} \right]^{1/2} = \left[\frac{iK}{6\pi\epsilon_0 r} \right]^{1/2} \quad (90)$$

or

$$dt = \left[\frac{6\pi\epsilon_0}{Ki} \right]^{1/2} r^{1/2} dr. \quad (91)$$

Upon integration, one obtains

$$\int_0^{t_{res}} dt = \left[\frac{6\pi\epsilon_0}{Ki} \right]^{1/2} \int_{r_0}^{r_1} r^{1/2} dr \quad (92)$$

$$t_{res} = \left[\frac{6\pi\epsilon_0}{Ki} \right]^{1/2} \frac{2}{3} (r_1^{3/2} - r_0^{3/2}) \quad (93)$$

or, if $r \gg r_0$,

$$t_{res} = \left[\frac{6\pi\epsilon_0}{Ki} \right]^{1/2} \frac{2}{3} r_1^{3/2} \quad (94)$$

$$= \left[\frac{8\pi\epsilon_0 r_1^3}{3Ki} \right]^{1/2} \quad (95)$$

Sampling ion density, ρ_{samp}

An expression for ion current density is

$$J = K\rho E. \quad (96)$$

At the exterior boundary of the spherical ion source, the ion density, ρ_1 , is

$$\rho_1 = \frac{J_1}{KE_1}, \quad (97)$$

where J_1 and E_1 are, respectively, the ion current density and field strength at the exterior surface of the ion source.

The ion current density, J_1 , is given by

$$J_1 = \frac{i}{4\pi r_1^2} \quad (98)$$

So, the ion density, ρ_1 , will become

$$\rho_1 = \frac{1}{K} \left[\frac{i}{4\pi r_1^2} \right] \left[\frac{6\pi\epsilon_0 K}{i} r_1 \right]^{1/2} \quad (99)$$

$$= \left[\frac{3i\epsilon_0}{8\pi K r_1^3} \right]^{1/2} \quad (100)$$

Applied potential, V_0

Again, the field strength, E , is

$$E = \left[\frac{i}{6\pi\epsilon_0 K} \frac{1}{r} \right]^{1/2} = \frac{dV}{dr} \quad (101)$$

Upon integration, an expression for applied potential is produced:

$$dV = \left[\frac{i}{6\pi\epsilon_0 K} \frac{1}{r} \right]^{1/2} dr \quad (102)$$

$$V_0 = \left[\frac{i}{6\pi\epsilon_0 K} \right]^{1/2} 2 (r_1^{1/2} - r_0^{1/2}) \quad (103)$$

APPENDIX C
COMPUTER PROGRAMS

Figure 40. SPACE.BAS: A program, written in VAX BASIC Version 3.3, used for the two dimensional modelling of ion sources.

```

1!*****
!*****
!*****
!*
!*      SPACE.BAS
!*      A simulation to model a two-dimensional
!*      space charge problem with cylindrical geometry.
!*
!*      WRITTEN BY DR. JAN SUNNER
!*      DEPT. OF CHEMISTRY
!*      MONTANA STATE UNIVERSTIY
!*
!*      AND      MARK BUSMAN
!*      DEPT. OF CHEMISTRY
!*      MONTANA STATE UNIVERSTIY
!*
!*****
!*****
!*****
!*
!*      LIST OF VARIABLES
!*      CONSTANTS:
!*      ZKAPPA: Ion mobility.
!*      EPS0: Permittivity
!*      COULC: 1/(4*pi*EPS0)
!*      TIME: (seconds)
!*      TTOT: Maximum for total elapsed time
!*      TSTEP: Movement timestep
!*      TSNAP: Timestep between "snapshots"
!*      TE: Time step between field calculations
!*      T: Time counter for elapsed time
!*      T2: Time counter for "snapshots"
!*      TC: Time counter for field recalc.
!*      TSTART: Initial time in program run.
!*
!*      CURRENT: (amps)
!*      ZJ0: Current at source
!*      CURR: Grid of current measured at surface
!*      QDC: Current injected in a given cell
!*
!*      GEOMETRY:
!*      GRID$ Indication of geometry type
!*      NCX No. of increments in x-direction
!*      NCY No. of increments in y-direction
!*      Q Tangent of angle in parabolic geo.
!*      CHARGE: (coulombs)
!*      QN Needle charge
!*      QD Injection charge
!*      QNUM Charge grid
!*      QSUMNUM Total charge of entire grid
!*      QGAPNUM Total charge of reduced (gap) grid
!*      Q Charge grid
!*      QCH Charge transfer matrix
!*      DISTANCES: (meters)
!*      FP: Distance of needle charge behind tip
!*      D: Distance between planes (SQ)
!*      D: Plane - needle tip distance (PARA)
!*      DP: Distance between cells par. to plates
!*      YNEEC: Distance between plate and needle tip
!*      RDIS: Maximum charge input radius
!*      RODIS: Minimum charge input radius
!*      RADMIN: Min. input rad. at resol. of grid
!*      RADMAX: Max. input rad. at resol. of grid
!*      RD: Distance between adjacent cells

```

Figure 40. SPACE.BAS-continued

```

!*          AD:      Distance between adjacent cells          *
!*          G:       Distance from focal point to plate       *
!*          COUNTERS:                                     *
!*          NNX:     Used to count loops working in x-dir     *
!*          NY:      Used to count loops working in y-dir     *
!*          MISC:                                          *
!*          ADIS     Maximum angle for current injection      *
!*          RDEG     Angular range in parabolic geometry      *
!*          FIDIS                                          *
!*          SN:      # of fld timesteps per move timestep    *
!*          FINP$:   Restart status identifier                *
!*          T1$:     Dummy variables to input nonessential    *
!*          T2$:     strings from disk files.                 *
!*          T3$:     " " " " " " " " " " " " " " " " " " " *
!*          T4$:     " " " " " " " " " " " " " " " " " " " *
!*          T5$:     " " " " " " " " " " " " " " " " " " " *
!*          Q1:      Terms in solution to quadratic form.    *
!*          Q2:      used for setting parabolic grid.         *
!*          ASTEP:   Angular increment in torus integr.       *
!*****
!Set up arrays, constants, etc.
2  DIM X(15,15), Y(15,15), EX(15,15), EY(15,15), DOUBLE QNUM(15,15)
3  DIM A(15), B(15), ANG(15), ANGR(15)
   DIM DOUBLE QCH(15,15), DOUBLE QD(15), DOUBLE QDC(15)
4  DIM SINGLE Q(15)
5  DIM RD(15,15,2,1), AD(15,15,2,1), DR(15,15), DA(15,15)
   DIM DOUBLE QSUMNUM(1), DOUBLE QGAPNUM(1)

!  INTEGER I-N
!  DOUBLE A-H, O-Z

ZKAPPA = 1E-4
EPS0 = 8.85E-12
COULC = 1/EPS0/4/PI

10 !input data - section
   INPUT "DO YOU WANT TO READ FROM FILE (Y/N) ", FZ$
   IF (FZ$="y" OR FZ$="n") !ASSURE SHIFT LOCK
   THEN
       PRINT "Set 'Caps Lock'"
       GOTO 10
   END IF
   INPUT "FILENAME ", FILE$
   IF FZ$="Y"
   THEN
       INPUT "STARTTIME/ms ", TS
       TSTART=TS*1E-3
       INPUT "TOTAL TIME/ms ", TS
       TTOT=TS*1E-3
       T2=0
       TC=0
       GOSUB 1000 !SNAPRI          FIND A FILE FOR RESTART OF PROGRAM
!TIMESTEPS
       PRINT "TSTEP      ", TSTEP    !MOVEMENT TIMESTEP
       PRINT "TSNAP      ", TSNAP    !"SNAPSHOT" TIMESTEP
       PRINT "T,E-field ", TE       !FIELD CALCULATION TIMESTEP
       PRINT "Disch. curr. ", ZJ0    !CURRENT
       INPUT "Change (Y/N) ", A$     !CHANGE ANY TIME PARAMETERS?
       IF A$="Y"
       THEN
           TSTEP2=TSTEP
           INPUT "TIME STEP,CURR/us ", TS
           TSTEP=TS*1E-6          !TIMESTEP MODIFICATIONS
           INPUT "TIME STEP,E-FIELD/us ", TS

```

Figure 40. SPACE.BAS-continued

```

TE=TS*1E-6
INPUT "TIME SNAP/us ", TS
TSNAP=TS*1E-6
END IF

GOSUB 1100 !SNAPR      READ THE SAVED FILE FOR FIELD DISTRIBUTIONS
PRINT T

!   IF T<(TSTART-1E-6) THEN GOTO 100 END IF
CLOSE #1
OPEN FILE$ FOR OUTPUT AS #1
FINP$="Y"
  T2=0
  TC=0
  PRINT "TSTART/s ", T
FOR NY=0 TO NCY+1
  CURR=0
  FOR NNX=0 TO NCX+1
    Q(NNX)=CSNG(QNUM(NNX,NY))
    Q(NNX)=QNUM(NNX,NY)
    PRINT NNX, NY, Q(NNX)
  NEXT NNX
  FOR NNX=1 TO NCX
    CURR=CURR+EY(NNX,NY)*ZKAPPA*Q(NNX)/(D/NCY)
  NEXT NNX
  PRINT "Current at NY= "; NY; " is "; CURR
!   INPUT "Pause ", P
NEXT NY

ELSE
  FINP$="N"

INPUT "Square or Parabolic grid system (SQ/PARA) ", GRID$
!DETERMIN THE GEOMETRY OF THE GRID SYSTEM
IF GRID$="PARA"      !PARABOLIC GEOMETRY
  THEN
    GOSUB 2800 !GRID
  ELSE
    GOSUB 2750 IF GRID$="SQ" !GRIDSQ---RECTANGULAR GEOMETRY
  END IF
!   INPUT "Print-out of coordinates (Y/N), printer on? ", A$
!   IF A$="Y" THEN GOSUB 2850 END IF GROUT
  INPUT "TIME STEP,CURR/us ", TS      !Input timestep parameters
  TSTEP=TS*1E-6
  INPUT "TIME STEP,E-FIELD/us ", TS
  TE=TS*1E-6
  INPUT "TIME SNAP/us ", TS
  TSNAP=TS*1E-6
  INPUT "TOTAL TIME/us ", TS
  TTOT=TS*1E-6
  INPUT "DISCHARGE CURRENT/ uA ", ZJ
  ZJ0=1e-6*ZJ      !to A
  T=0
  T2=0
  TC=0
  FINP$="N"
  GOSUB 1400 !CHINF
END IF
IF GRID$="SQ"
  THEN
    !INPUT PARAMETERS PERTINENT TO RECTANGULAR
    !GEOMETRY
    INPUT "NEEDLE CHARGE ", QN
    INPUT "DISTANCE BEHIND PLATE/mm ", FP0
    FP=FP0/1000
    YNEEC=D+FP
  ELSE
    IF GRID$="PARA"      !INPUT PARAMETERS PERTINENT TO PARABOLIC

```

Figure 40. SPACE.BAS-continued

```

      THEN                      !GEOMETRY
      INPUT "NEEDLE CHARGE ", QN
      INPUT "DISTANCE BEHIND PLATE/mm ", FP0
      FP=FP0/1000
      YNEEC=D+FP
      END IF
    END IF
    GOSUB 1500 !CHINP2
    DNSUM=0
    FOR NNX=1 TO NCX
      DNSUM=DNSUM+QD(NNX)
    NEXT NNX
    PRINT "DNSUM= ", DNSUM

    IF FINP$="Y"
    THEN
      IF GRID$="PARA" THEN GOSUB 2800 END IF !GRID
      IF GRID$="SQ" THEN GOSUB 2750 END IF !GRIDSQ
      GOSUB 2820 !DIST
      GOSUB 2100 !EFLD
      FIRST$="Y"
      LT=1
      GOTO 300
    END IF
    FIRST$="N"
    GOSUB 2820 !DIST
    SN=TE/TSTEP
    T=TE
    GOSUB 1600 !CHINJ
    GOSUB 1200 !SNAPINI
    GOSUB 2100 !EFLD

    !time stepping
300  T=T+TSTEP
    T2=T2+TSTEP
    TC=TC+TSTEP
    PRINT "T= ", T
    IF T>(TTOT+1E-10)
    THEN
      GOSUB 2260 !SNAP
      PRINT "THIS IS THE END!!!"
      PRINT
      GOTO 3000
    ELSE
      SN=1
      GOSUB 1600 !CHINJ
      IF TC>(TE-(1E-10))
      THEN
        TC=TC-TE
        PRINT "Q-sum ", QSUMNUM
        PRINT "Q-gap ", QGAPNUM
        IF FIRST$="N" THEN GOSUB 2100 END IF !EFLD
        FIRST$="N"
        LT=1
      END IF
      IF T2>(TSNAP-(1E-10))
      THEN
        T2=T2-TSNAP
        TMU=T*1E6
        PRINT "Snap output to file"
        PRINT "T/us= ", TMU
        GOSUB 2260 !SNAP
      END IF
      GOSUB 2000 !CURR
      GOSUB 1900 !NEWCH
    
```

```

*****
***** SUBROUTINE SECTION *****
*****
***** LIST OF SUBROUTINES *****
*****
CHCPOUT
LOCATED BY USING GOSUB 1800

CHINI Charge initiation
LOCATED BY USING GOSUB 1300

CHINJ Injects charges into first cell line
LOCATED BY USING GOSUB 1600

CHINP Calculate injected charges into first cell line
LOCATED BY USING GOSUB 1400

CHINP2 Converts injection current to injected charge
LOCATED BY USING GOSUB 100

CURR Calculates charge transfer matrix
LOCATED BY USING GOSUB 2000

DIST Calculates intercell distances
LOCATED BY USING GOSUB 2820

EFLD Electric field calculation
LOCATED BY USING GOSUB 2100

GRID Geometry input and cell coordinate calculation
LOCATED BY USING GOSUB 2800

GRIDSQ Same as GRID but for square grid system
LOCATED BY USING GOSUB 2750

GOUT Output to screen of geometry and coordinates
LOCATED BY USING GOSUB 2900

NEWCH Calculates new charge distribution
LOCATED BY USING GOSUB 1900

RINGINT Integration of the charge in any ring
GOSUB 2500

RINGSAME Integration of the charge in the same ring
as a selected cell
LOCATED BY USING GOSUB 2400

RINTX
LOCATED BY USING GOSUB 2700

RINTY
LOCATED BY USING GOSUB 2600

SNAP Writes snap-information to file
LOCATED BY USING GOSUB 2260

```

Figure 40. SPACE.BAS-continued

```

!
!      SNAPINI Initiates SNAP-file for output, writes input parameters
!      LOCATED BY USING GOSUB 1200
!
!      SNAPR  Reads electric field and charge distribution from SNAP file
!      LOCATED BY USING GOSUB 1100
!
!      SNAPRI  Reads data-head from SNAP-file
!      LOCATED BY USING GOSUB 1000
!
!*****
!*****
1000
!*****
!*****
!SNAPRI - subroutine
!read data-head from SNAP-file
!*****
!*****

      OPEN FILE$ FOR INPUT AS #1      !to disk
      INPUT #1, GRID$                !geometry type
      INPUT #1, T1$                  !"point-to-plane corona"
      IF GRID$="SQ"                  !square geometry
      THEN
        PRINT "Square coordinate system"
        INPUT #1, D, DP, NCY, NCX, ADIS      !input square parameters
      ELSE
        IF GRID$="PARA"
        THEN
          INPUT #1, D, FP, NCY, NCX, RDEG      !input parabolic parameters
        END IF
      END IF
      INPUT #1, TSNAP, TE, TSTEP, TTOT2
      INPUT #1, ZJ0
      FOR NNX=1 TO NCX
        INPUT #1, QDC(NNX)
      NEXT NNX
      RETURN

1100
!*****
!*****
!SNAPR - subroutine
!input of electric field distribution from SNAP file
!*****
!*****

      !ERROR TRAP
      ON ERROR GOTO 1150
      WHILE 0=0
        INPUT #1, T2$, T      !"T= "
        PRINT "T ", NS, T
        INPUT #1, T3$          !"ELECTRIC FIELD AND CHARGE DISTRIBUTIONS"
        INPUT #1, T4$, QSUMNUM !"Q,sum= "
        INPUT #1, T5$, QGAPNUM !"Q,gap= "
        QS(NS)=CSNG(QSUMNUM)
        QSG(NS)=CSNG(QGAPNUM)
        FOR NY=1 TO NCY
          FOR NNX=1 TO NCX
            INPUT #1, I, J, EX(NNX,NY), EY(NNX,NY), QT

            QNUM(NNX,NY)=CDBL(QT)
            QNUM(NNX,NY)=QT
            PRINT I,J, EX(NNX,NY), QNUM(NNX,NY)
          NEXT NNX
        NEXT NY
        NNX=0

```

Figure 40. SPACE.BAS-continued

```

      FOR NY=0 TO NCY+1
      INPUT #1, I, J, QT
      QNUM(NNX,NY)=CDBL(QT)
      QNUM(NNX,NY)=QT
      NEXT NY
      NNX=NCX+1
      FOR NY=0 TO NCY+1
      INPUT #1, NNX, NY, QT
      QNUM(NNX,NY)=CDBL(QT)
      QNUM(NNX,NY)=QT
      NEXT NY
      NY=0
      FOR NNX=1 TO NCX
      INPUT #1, NNX, NY, QT
      QNUM(NNX,NY)=CDBL(QT)
      QNUM(NNX,NY)=QT
      NEXT NNX
      NY=NCY+1
      FOR NNX=1 TO NCX
      INPUT #1, NNX, NY, QT
      QNUM(NNX,NY)=CDBL(QT)
      QNUM(NNX,NY)=QT
      NEXT NNX
      NEXT !WHILE
1150 IF ERR=11 THEN RESUME 1160 ELSE ON ERROR GOTO 0
1160 RETURN

1200
!*****
!*****
!SNAPINI - subroutine
!initialize SNAP-file
!*****

      OPEN FILE$ FOR OUTPUT AS #1
      IF GRID$="PARA"
      THEN
        PRINT #1, GRID$                      !Geometry type
        PRINT #1, "Point-to-plane corona"
        PRINT #1, D; ", "; FP; ", "; NCY; ", "; NCX; ", "; RDEG !PARA geometry p
arameters
      ELSE
        IF GRID$="SQ"
        THEN
          PRINT #1, GRID$
          PRINT #1, "Plane-to-plane corona"
          PRINT #1, D; ", "; DP; ", "; NCY; ", "; NCX; ", "; ADIS !SQ geometry par
ameters
        END IF
      END IF
      PRINT #1, TSNAP; ", "; TE; ", "; TSTEP; ", "; TTOT      !Time parameters
      PRINT #1, ZJ0                      !Current
      FOR NNX=1 TO NCX
      PRINT #1, QDC(NNX)
      NEXT NNX
      CLOSE #1
      RETURN

1300
!*****
!*****
!CHINI - subroutine
!charge distribution initiated
!*****

      INPUT "Charge on needle ", QN

```

Figure 40. SPACE.BAS-continued

```

PRINT "Charge initiation"
!FOR NY=1 TO NCY
!FOR NNX=1 TO NCX
!QNUM(1,5)=1D-12
!QNUM(3,5)=0D-12
!QNUM(4,5)=0D-12

!NEXT NNX
!NEXT NY

RETURN

1400
!*****
!*****
!CHINP - subroutine
!calculate injected charges into first cell line
!*****
PRINT "Calculates injecting charges"
N=0
NY=NCY
!
** CHARGE INJECTION FOR PARABOLIC GEOMETRY **
IF GRID$="PARA"
THEN
INPUT "CURRENT INJECTION ANGLE/deg ", ADISI
ADIS=ADISI/180*PI !max angle for discharge current
FIDIS=1-COS(ADIS) !steradians/2/pi
FOR NNX=1 TO NCX
IF N=1
THEN
QDC(NNX)=0
ELSE
IF NNX=1
THEN
A1=0
ELSE
A1=ANGR(NNX)-ASTEPR/2
END IF
A2=ANGR(NNX)+ASTEPR/2
IF A2>ADIS
THEN
A2=ADIS
N=1
ELSE
QDC(NNX)=(COS(A1)-COS(A2))/FIDIS*ZJ0
END IF
END IF
NEXT NNX
ELSE
!
** CHARGE INJECTION FOR SQUARE GEOMETRY **
IF GRID$="SQ"
THEN
INPUT "MAXIMUM CHARGE INPUT RADIUS/mm ", RDIS0 !Define ring for
RDIS=RDIS0/1000 !injection of charge
INPUT "MINIMUM CHARGE INPUT RADIUS/mm ", RODIS0
RODIS=RODIS0/1000

TOTS=PI*(RDIS*RDIS-RODIS*RODIS) !Total area of injection ring
FOR NNX=1 TO NCX
IF N=1
THEN
QDC(NNX)=0
ELSE
IF (NNX-0.5)*DP<RDIS !Radius inside of ring's outer boundary?
THEN

```

Figure 40. SPACE.BAS-continued

```

        RADMAX=(NNX-0.5)*DP
    ELSE
        RADMAX=RODIS
        N=1
    END IF
    IF NNX=1
    THEN
        RADMIN=0
    ELSE
        RADMIN=(NNX-1.5)*DP
    END IF
    IF RADMIN<RODIS !Radius inside of ring's inner boundary?
    THEN
        IF RADMAX<RODIS
        THEN
            RADMIN=RADMAX
        ELSE
            RADMIN=RODIS
        END IF
    END IF
    QDC(NNX)=PI*(RADMAX*RADMAX-RADMIN*RADMIN)/TOTS*ZJO
        !Current in a cell is the total injection current
        !multiplied by the ratio of the cell's area to the
        !total area of the injection ring.
    END IF
NEXT NNX
END IF
END IF
FOR NNX=1 TO NCX
PRINT QDC(NNX)
NEXT NNX
RETURN

1500
!*****
!*****
!CHINP2 - subroutine
!Converts injection current to injected charge
!*****
        FOR NNX=1 TO NCX
            QD(NNX)=QDC(NNX)*TSTEP !Charge injected in a cell is current
                                   !multiplied by length of movement timestep.
        NEXT NNX
    RETURN

1600
!*****
!*****
!CHINJ - subroutine
!discharge charge input
!*****
        FOR NNX=1 TO NCX
            QNUM(NNX,NCY)=QNUM(NNX,NCY)+SN*QD(NNX) !Puts injected charge into
                                                    !charge grid
        NEXT NNX
    RETURN

1900
!*****
!*****
!NEWCH - subroutine
!calculates new charge distribution
!*****

```

Figure 40. SPACE.BAS-continued

```

QSUMNUM=0
QGAPNUM=0
PRINT "New charge distribution calculated"
FOR NY=0 TO NCY+1
  FOR NNX=0 TO NCX+1
    QNUM(NNX,NY)=QNUM(NNX,NY)+QCH(NNX,NY)
    !Add movement charge to existing charge
    QSUMNUM=QSUMNUM+QNUM(NNX,NY)
    !Total charge of entire grid
    PRINT QNUM(NNX,NY), QCH(NNX,NY)
  NEXT NNX
NEXT NY
FOR NY=1 TO NCY
  FOR NNX=1 TO NCX
    QGAPNUM=QGAPNUM+QNUM(NNX,NY)
    !Total charge of "gap" grid
  NEXT NNX
NEXT NY

!PRINT "TOTAL CHARGES ", QGAPNUM, QSUMNUM
RETURN

2000
!*****
!CURR -subroutine
!calculation of charge transfer between cells
!*****

!*****
!***** LOCAL VARIABLE DESCRIPTIONS *****
!*****
!CHARGE:
!      QCH: Charge transfer matrix
!      QL: Charge moving to left
!      QR: Charge moving to right
!      QU: Charge moving up
!      QD: Charge moving down
!      QUL: Charge moving up and to left
!      QUR: Charge moving up and to right
!      QDL: Charge moving down and to left
!      QDR: Charge moving down and to right
!      QLEAVE: Total charge leaving a cell
!      Q: Charge of a cell from which charge is being
!          moved.
!
!VELOCITY:
!      VR: Radial velocity
!      VA: Angular velocity
!
!DISTANCE:
!      DR: Grid for radial distance travelled by a cell.
!      RW: Radial "width" of a cell
!      RC: Radial distance travelled by a cell
!      RU: Radial distance travelled by the cell "up"
!          in the grid.
!      RD: Radial distance travelled by the cell "down"
!          in the grid.
!      RDB: Average distance travelled by a cell and
!          the cell "down" in the grid.
!      RUB: Average distance travelled by a cell and
!          the cell "up" in the grid.
!      RWN: Radial distance travelled by a cell with
!          compensation for "expansion."
!      DA: Grid for axial distance travelled by a cell
!      AW: Axial "width" of a cell
!      AC: Axial distance travelled by a cell
!      AR: Axial distance travelled by the cell to the

```

Figure 40. SPACE.BAS-continued

```

!
!           right.
!           AL:   Axial distance travelled by the cell to the
!                 left.
!           ALB:  Average distance travelled by a cell and
!                 the cell to the left.
!           ARB:  Average distance travelled by a cell and
!                 the cell to the right.
!           AWN:  Axial distance travelled by a cell with
!                 compensation for "expansion."
!
!           FIELD:
!           ER:   Radial component of field
!           EA:   Angular component of field
!           CHARGE/FRACTION:
!           QFU:  Fraction of charge moving up.
!           QFD:  Fraction of charge moving down.
!           QFR:  Fraction of charge moving to the right.
!           QFL:  Fraction of charge moving to the left.
!           QFM:  Maximum fraction of charge moving.
!
!*****
!*****
!
!           PRINT "Charge transfer/current calculated"
!           ERASE QCH
!           FOR NY=0 TO NCY+1
!             FOR NNX=0 TO NCX+1
!               QCH(NNX,NY)=0
!             NEXT NNX
!           NEXT NY
!
!           QMAX=0
!           FOR NY=1 TO NCY           !choose cell
!             FOR NNX=1 TO NCX
!
!               !calculate radial electric field
!               ER=(-RD(NNX,NY,0,0)*EX(NNX,NY)-RD(NNX,NY,1,0)*EY(NNX,NY))/RD(NNX,NY,2,0)
!
!               !calculate axial electric field
!               EA=(-RD(NNX,NY,1,0)*EX(NNX,NY)+RD(NNX,NY,0,0)*EY(NNX,NY))/RD(NNX,NY,2,0)
!
!               IF NNX=1 THEN EA=0 END IF
!               VR=ZKAPPA*ER           !radial velocity
!               VA=ZKAPPA*EA           !axial velocity
!               DR(NNX,NY)=VR*TSTEP     !distance of radial travel for cell center
!               DA(NNX,NY)=VA*TSTEP     !distance of axial travel for cell center
!
!             NEXT NNX
!           NEXT NY
!
!           FOR NNX=1 TO NCX
!             FOR NY=1 TO NCY
!
!               !fraction of charge exiting left and right
!               IF NNX=1                 !On edge of grid
!                 THEN
!                   RI=AD(NNX,NY,2,1)/2
!                   RF=RI+DA(NNX+1,NY)/2
!                   QFR=(RF*RF/RI/RI-1)
!                   QFL=0
!                 ELSE
!                   !Mechanism for the axial "expansion" of a cell in response
!                   !to movement of charge in neighboring cells.
!                   AW=AD(NNX,NY,2,1)
!                   AC=DA(NNX,NY)       !Axial velocities
!                   AL=DA(NNX-1,NY)
!                   IF NNX=NCX           !On outer edge
!                     THEN

```

Figure 40. SPACE.BAS-continued

```

        AR=2*AD-AL
    ELSE
        AR=DA (NNX+1,NY)
    END IF
    ALB=(AL+AC)/2
    ARB=(AR+AC)/2
    AWN=AW-ALB+ARB
    IF ALB<0 THEN QFL=-ALB/AWN ELSE QFL=0 END IF
    IF ARB>0 THEN QFR=ARB/AWN ELSE QFR=0 END IF
END IF

!fraction of charge exiting up and down
RW=RD (NNX,NY,2,0)      !Distance
RC=DR (NNX,NY)          !Radial distance.
IF NY=NCY                !Same 'slice' of grid?
THEN
    !Mechanism for the radial "expansion" of a cell in response
    !to movement of charge in neighboring cells.
    RUB=0
ELSE
    RU=DR (NNX,NY+1)      !Radial distance.
    RUB=(RU+RC)/2
END IF
IF NY=1
THEN
    RDB=2*RC-RU
ELSE
    RD=DR (NNX,NY-1)      !Radial distance.
    RDB=(RD+RC)/2
END IF
RWN=RW+RUB-RDB
IF RUB>0 THEN QFU=RUB/RWN ELSE QFU=0 END IF      !Charge up
IF RDB<0 THEN QFD=-RDB/RWN ELSE QFD=0 END IF    !Charge down
!testing for Q-max
IF QFU>QMAX      !Monitor fraction of movement--up
THEN
    QMAX=QFU
    NID=1        !Indicate the direction of maximum movement
    NXM=NNX
    NYM=NY
END IF
IF QFR>QMAX      !Monitor fraction of movement--right
THEN
    QMAX=QFR
    NID=2
    NXM=NNX
    NYM=NY
END IF
IF QFD>QMAX      !Monitor fraction of movement--down
THEN
    QMAX=QFD
    NID=3
    NXM=NNX
    NYM=NY
END IF
IF QFL>QMAX      !Monitor fraction of movement--left
THEN
    QMAX=QFL
    NID=4
    NXM=NNX
    NYM=NY
END IF

!
Q=CSNG (QNUM (NNX,NY))
Q=QNUM (NNX,NY)

```

Figure 40. SPACE.BAS-continued

```

      QL=QFL*(1-QFU-QFD)*Q      !Charge going left from cell
      QR=QFR*(1-QFU-QFD)*Q      !Charge going right from cell
      QU=QFU*(1-QFL-QFR)*Q      !Charge going up from cell
      QD=QFD*(1-QFL-QFR)*Q      !Charge going down from cell
      QUL=QFU*QFL*Q             !Charge going up and left from cell
      QUR=QFU*QFR*Q             !Charge going up and right from cell
      QDL=QFD*QFL*Q             !Charge going down and left from cell
      QDR=QFD*QFR*Q             !Charge going up and left from cell
      QLEAVE=(QL+QR+QU+QD+QUL+QUR+QDL+QDR) !Charge leaving cell
      !Transfer movement information to a "movement" matrix
      QCH(NNX,NY)=QCH(NNX,NY)-QLEAVE
      QCH(NNX+1,NY)=QCH(NNX+1,NY)+QR
      QCH(NNX-1,NY)=QCH(NNX-1,NY)+QL
      QCH(NNX,NY+1)=QCH(NNX,NY+1)+QU
      QCH(NNX,NY-1)=QCH(NNX,NY-1)+QD
      QCH(NNX-1,NY-1)=QCH(NNX-1,NY-1)+QDL
      QCH(NNX+1,NY-1)=QCH(NNX+1,NY-1)+QDR
      QCH(NNX-1,NY+1)=QCH(NNX-1,NY+1)+QUL
      QCH(NNX+1,NY+1)=QCH(NNX+1,NY+1)+QUR

      NEXT NY
      NEXT NNX

      IF LT=1
      THEN
        PRINT "Q-max ", QMAX, NID, NXM, NYM
        FOR I=1 TO 100
          N=I
          NEXT I
          LT=0
        END IF
        IF QMAX>0.05      !Is maximum movement over the set threshold?
        THEN
          PRINT "WARNING, Q,max= ", QMAX, NID      !Display movement
          PRINT "TIME ", T, NNX, NY              !warning
          WARN$ = "Y"
        END IF
      RETURN

2100
!*****
!*****
!EFLD - subroutine
!for calculation of electric field
!*****

!returns electric field vector in each cell
PRINT "Calculation of E-field"
FOR NY=1 TO NCY      !cell for which electric field is to be calc.
FOR NNX=1 TO NCX
!NY=2: NNX=2
!PRINT "NNX, NY ", NNX, NY
  EX=0
  EY=0
  DS=X(NNX,NY)      !x-coordinate of cell
  Y1=Y(NNX,NY)      !y-coordinate of cell
!
! special treatment for axial cells???
  FOR KY=1 TO NCY      !charged torus to be interacted with cell
  FOR KX=1 TO NCX
    L=0
!
!   QNUM(KX,KY)=1E-6
!
!   IF (KX=1 AND NNX=1 AND NY=KY) THEN GOTO 2150 END IF
    DR=X(KX,KY)      !x-coordinate for torus
    Y2=Y(KX,KY)      !y-coordinate for torus
    Q=QNUM(KX,KY)      !charge for torus
    DL=Y2-Y1          !Distance between cell and torus (y-comp.)

```

Figure 40. SPACE.BAS-continued

```

      DL2=Y2+Y1      !Distance between cell and "mirror torus"(y-cp.)
      NSTEP=20
      IF (KX=NNX AND KY=NY) !Is the cell contained in the torus?
      THEN          !same torus interaction
      PRINT KX, NNX, KY, NY
      IF NNX=1
      THEN
      EXT=0          !Define E-fld for "same torus" and first row
      EYT=0
      EXM=0
      EYM=-COULC*Q/DL2/DL2
      ELSE
      GOSUB 2400 !RINGSAME      Define E-fld for "same torus"
      L=1
      GOSUB 2500 !RINGINT
      L=0
      END IF
      ELSE
      GOSUB 2500 !RINGINT      integrates coulomb over charged torus
      !returns ey2 and ex2
      END IF
      EX=EX+EXT+EXM          !x-component of E-fld in a cell is the
      !sum of the previous value of E-fld, the
      !x-component from the torus and the
      !x-component from the "mirror torus"
      EY=EY+EYT+EYM          !y-component of E-fld in a cell is the
      !sum of the previous value of E-fld, the
      !y-component from the torus and the
      !y-component from the "mirror torus"

! IF (KX=1 AND KY=4)
! THEN
! PRINT NNX, NY
! PRINT "E,T-CHARGE ", KX, KY, EXT, EYT
! PRINT "E,MIRROR-CH", KX, KY, EXM, EYM
! END IF
2150      NEXT KX      !Continue with an interaction with another torus
      NEXT KY
      !electric field from needle charge
      DYN=YNEEC-Y(NNX,NY)      !y-component of distance from needle
      DXN=X(NNX,NY)            !x-component of distance from needle
      DN2=DYN*DYN+DXN*DXN
      DN=SQR(DN2)              !Distance from needle
      EXN=COULC*QN/DN2*DXN/DN      !x-component of E-fld from needle
      EYN=-COULC*QN/DN2*DYN/DN      !y-component of E-fld from needle
      !electric field from needle mirror charge
      DYNM=YNEEC+Y(NNX,NY)      !y-component of distance
      !from "mirror needle"
      DNM2=DYNM*DYNM+DXN*DXN
      DNM=SQR(DNM2)              !distance from "mirror needle"
      EXNM=-COULC*QN/DNM2*DXN/DNM      !x-component of E-fld from
      !"mirror needle"
      EYNM=-COULC*QN/DNM2*DYNM/DNM      !y-component of E-fld from
      !"mirror needle"

! PRINT NNX,NY
! PRINT "NEEDLE ", EXN, EYN
! PRINT "MIRROR ", EXNM, EYNM

      EX(NNX,NY)=EX+EXN+EXNM      !x-component of E-fld in a cell is the
      !sum of the previous value of E-fld, the
      !x-component from the needle and the
      !x-component from the "mirror needle"
      EY(NNX,NY)=EY+EYN+EYNM      !y-component of E-fld in a cell is the
      !sum of the previous value of E-fld, the
      !y-component from the needle and the
      !y-component from the "mirror needle"

```

Figure 40. SPACE.BAS-continued

```

1      QT=CSNG(QNUM(NNX,NY))
      QT=QNUM(NNX,NY)
      PRINT NNX, NY, EX(NNX,NY), EY(NNX,NY), QT

      NEXT NNX                !next cell
      NEXT NY
      RETURN

2260
!*****
!*****
!SNAP - subroutine
!output of electric field distribution to hard disc
!*****

1      OPEN FILES FOR OUTPUT AS #1,ORGANIZATION SEQUENTIAL FIXED !&
1      ACCESS APPEND

                                !Reopen existing file
                                !Send the current time
      PRINT #1, "T= "; ", "; T
      PRINT #1, "ELECTRIC FIELD AND CHARGE DISTRIBUTIONS"
      PRINT #1, "Qsum= "; ", "; QSUMNUM          !Sum of charges in geometry
      PRINT #1, "Qgap= "; ", "; QGAPNUM          !Sum of charges in "reduced geom
etry"

      FOR NY=1 TO NCY
      FOR NNX=1 TO NCX
1      QT=CSNG(QNUM(NNX,NY))
      QT=QNUM(NNX,NY)
      PRINT #1, NNX; ", "; NY; ", "; EX(NNX,NY); ", "; EY(NNX,NY); ", "; QT
                                !Store cell "x-identifier," cell "y-identifier,"
                                !x-component of E-fld, y-component of E-fld,
                                !and the charge in the cell.

      NEXT NNX
      NEXT NY
      NNX=0
      FOR NY=0 TO NCY+1
1      QT=CSNG(QNUM(NNX,NY))
      QT=QNUM(NNX,NY)
      PRINT #1, NNX; ", "; NY; ", "; QT
                                !Store cell "x-identifier," cell "y-identifier,"
                                !and the charge in the cell.

      NEXT NY
      NNX=NCX+1
      FOR NY=0 TO NCY+1
1      QT=CSNG(QNUM(NNX,NY))
      QT=QNUM(NNX,NY)
      PRINT #1, NNX; ", "; NY; ", "; QT
      NEXT NY
      NY=0
      FOR NNX=1 TO NCX
1      QT=CSNG(QNUM(NNX,NY))
      QT=QNUM(NNX,NY)
      PRINT #1, NNX; ", "; NY; ", "; QT
      NEXT NNX
      NY=NCY+1
      FOR NNX=1 TO NCX
1      QT=CSNG(QNUM(NNX,NY))
      QT=QNUM(NNX,NY)
      PRINT #1, NNX; ", "; NY; ", "; QT
      NEXT NNX
1      CLOSE #1
      RETURN

2400
!*****
!*****
!RINGSAME - subroutine

```

Figure 40. SPACE.BAS-continued

```

!numerical integration for same ring
!*****

      Z=(NNX-1)*2
      ALIM0=ATN(1/SQR(Z*Z-1))      !Integration limits.
      ALIM1=PI
      ASTEP=(ALIM1-ALIM0)/NSTEP    !Increment for integration.
      ALM0=ALIM0+ASTEP/2           !Middle of first increment.
      SUM=0                         !Zero the "projection" counter.
      FOR I=1 TO NSTEP             !Loop for integration.
      ALFA=ALM0 + (I-1)*ASTEP      !Angle for integration.
      FUNC=1/SQR(1-COS(ALFA))      !"Projection" function.
      SUM=SUM+FUNC*ASTEP           !Sum of "projection."
      NEXT I
      EXT=COULC*Q/PI/DR/DR/2.828427*SUM  !x-component of field.
      EYT=0                        !Field has no y-component.
      RETURN

2500
!*****
!RINGINT - subroutine
!numerical integration of the interaction with charged ring
!*****

      ALIM0=0                      !Initial angle for integration
      ALIM1=PI                     !Final angle for integration
      ASTEP=(ALIM1-ALIM0)/NSTEP    !Angle increment for integration
      ALM0=ALIM0+ASTEP/2           !Middle of first increment
      TR=DR                        !x-coordinate of cell giving the field.
      ROFF=DS                      !x-coordinate of the cell which the field acts on.
      IF L=1 THEN GOTO 2550 END IF  !Mirror charge only?
      Y=DL                         !y-component of distnace between cells.
      GOSUB 2600 !RINTY
      EYT=-COULC*Q*Y/PI*SUM        !y-component of field from torus.
      GOSUB 2700 !RINTX
      EXT=-COULC*Q/PI*SUM          !x-component of field from torus.
2550  Y=DL2
      GOSUB 2600 !RINTY
      EYM=-COULC*Q*Y/PI*SUM        !y-component of field from mirror charge.
      GOSUB 2700 !RINTX
      EXM=COULC*Q/PI*SUM          !x-component of field from mirror charge.
      RETURN

2600
!*****
!RINTY - subroutine
!
!*****

      SUM=0
      FOR I=1 TO NSTEP             !Loop for angle incrementing
      ALFA=ALM0 + (I-1)*ASTEP      !Angle for integration
      FUNC=1/(Y*Y+ROFF*ROFF+TR*TR-2*TR*ROFF*COS(ALFA))^(3/2)
      SUM=SUM+FUNC*ASTEP           !Total y-projection
      NEXT I
      RETURN

2700
!*****
!RINTX - subroutine
!
!*****

```

Figure 40. SPACE.BAS-continued

```

SUM=0
FOR I=1 TO NSTEP
  ALFA=ALM0 + (I-1)*ASTEP
  !Loop for angle incrementing
  !Angle for integration
FUNC=(TR*COS(ALFA)-ROFF)/(Y*Y+ROFF*ROFF+TR*TR-2*TR*ROFF*COS(ALFA))^(3/2)
  !x-projection for increment
SUM=SUM+FUNC*ASTEP
  !Total x-projection
ADEG=ALFA/PI*180
NEXT I
RETURN

2750
!*****
!GRIDSQ - subroutine
!square grid system
!*****
IF FINP$="N"
THEN
  INPUT "Plane to plane distance/mm ", D0
  D=D0/1000
  INPUT "Number of cell lines parallel to planes ", NCY
  INPUT "Number of cell lines perpend. to planes ", NCX
  INPUT "Distance between these cell lines/mm ", DP0
  DP=DP0/1000
  GRID$="SQ"
END IF
NCT=NCY*NCX
PRINT "Total number of cells ", NCT
FOR NY=0 TO NCY-1
  FOR NNX=0 TO NCX-1
    X(NNX,NY)=DP*(NNX-1)
    Y(NNX,NY)=(D/NCY)*(NY-0.5)
    !x-coordinate for each cell
    !y-coordinate for each cell
  NEXT NNX
NEXT NY
RETURN

2800
!*****
!GRID - subroutine
!to set up parabolic grid system
!*****
IF FINP$="N"
THEN
  !Restart status
  INPUT "Tip to plane distance/mm ", D0
  D=D0/1000
  INPUT "Focal point to tip/mm ", FP0
  FP=FP0/1000
  INPUT "Number of parabola cell lines ", NCY
  INPUT "Number of radial grid cells ", NCX
  INPUT "Angular range, from 0 deg to ", RDEG
  ERASE QNUM
END IF
P=1/(4*FP)
YNEEC=D+FP
NCT=NCY*NCX
PRINT "Total number of cells ", NCT
ASTEP=RDEG/(NCX-1)
  !Angle increment in degrees.
ASTEPR=ASTEP/180*PI
  !Angle increment in radians.
!Find parabola constants for an equation y = ax^2 + b.
FOR NY=1 TO NCY
  B(NY)=D/NCY*(NY-0.5)

```

Figure 40. SPACE.BAS-continued

```

      A(NY)=1/4/(D+FP-B(NY))
NEXT NY
      A(0)=0
      B(0)=0
      B(NCY+1)=D
      A(NCY+1)=1/4/FP
FOR NNX=0 TO NCX+1
      ANG(NNX)=(NNX-1)*ASTEP           !Angle in degrees.
      ANGR(NNX)=ANG(NNX)/180*PI       !Angle in radians.
NEXT NNX
!
GOSUB 2850 GROUT
!cell coordinates
FOR NNX=0 TO NCX+1           !Increment angle.
      Q=TAN(ANGR(NNX))
FOR NY=1 TO NCY+1           !Increment parabola being described.
      IF ABS(Q)<1E-10
      THEN
          Y(NNX,NY)=B(NY) !y-coordinate for each cell
          X(NNX,NY)=0      !x-coordinate for each cell
      ELSE
          C=A(NY)*Q*Q
          G=D+FP !Total distance from focal pt. to plane.
          Q1=-(1/C+2*G) !1st constant in quadratic equation.
          Q2=G*G+B(NY)/C !2nd constant in quadratic equation.
          !y-coordinate is determined by solving a quadratic equation.
          Y=-Q1/2-SQR(Q1*Q1/4-Q2) !y-coordinate for each cell
          !x-coordinate is determined by substituting the y-coordinate
          !into the equation y = ax^2 + b.
          X=SQR((Y-B(NY))/A(NY)) !x-coordinate for each cell
          Y(NNX,NY)=Y
          X(NNX,NY)=X
      END IF
NEXT NY
NEXT NNX
FOR NY=1 TO NCY+1
      Y(0,NY)=Y(2,NY)
      X(0,NY)=-X(2,NY)
NEXT NY
FOR NNX=0 TO NCX+1
      Y(NNX,0)=0
      X(NNX,0)=TAN(ANGR(NNX))*(D+FP)
NEXT NNX
GRID$="PARA"
RETURN
2820
!*****
!DIST - subroutine
!"CALCULATES INTER-CELL DISTANCES"
!*****
PRINT "CALCULATES INTER-CELL DISTANCES"
FOR NY=1 TO NCY
FOR NNX=1 TO NCX
RD(NNX,NY,0,0)=X(NNX,NY-1)-X(NNX,NY)
RD(NNX,NY,0,1)=X(NNX,NY+1)-X(NNX,NY)
RD(NNX,NY,1,0)=Y(NNX,NY-1)-Y(NNX,NY)
RD(NNX,NY,1,1)=Y(NNX,NY+1)-Y(NNX,NY)
RD(NNX,NY,2,0)=SQR(RD(NNX,NY,0,0)^2+RD(NNX,NY,1,0)^2)
RD(NNX,NY,2,1)=SQR(RD(NNX,NY,0,1)^2+RD(NNX,NY,1,1)^2)
AD(NNX,NY,0,0)=X(NNX-1,NY)-X(NNX,NY)
AD(NNX,NY,0,1)=X(NNX+1,NY)-X(NNX,NY)
AD(NNX,NY,1,0)=Y(NNX-1,NY)-Y(NNX,NY)
AD(NNX,NY,1,1)=Y(NNX+1,NY)-Y(NNX,NY)
AD(NNX,NY,2,0)=SQR(AD(NNX,NY,0,0)^2+AD(NNX,NY,1,0)^2)

```

Figure 40. SPACE.BAS-continued

```

      AD(NNX,NY,2,1)=SQR(AD(NNX,NY,0,1)^2+AD(NNX,NY,1,1)^2)
      NEXT NNX
      NEXT NY
!      NNX=3: NY=3
      RETURN

2900
!*****
!*****
!GOUT - subroutine
!output of grid-points
!*****

      PRINT "PARABOLIC CONSTANTS"
      PRINT "NUMBER OF CELLS ", NCX, " TIMES ", NCY
      PRINT "      I          A(I)          B(I)"
      FOR NY=1 TO NCY
      PRINT NY, A(NY), B(NY)
      NEXT NY
      PRINT "J          ANG(J)          TAN(ANG(J))"
      FOR NNX=1 TO NCX
      PRINT NNX, ANG(NNX), TAN(ANG(NNX))
      NEXT NNX
      PRINT
      PRINT "PARABOLIC GRID POINTS "
      PRINT " J          X          L          Y"
      FOR NNX=1 TO NCX
      FOR NY=1 TO NCY
      YM=Y(NNX,NY)*1000
      XM=X(NNX,NY)*1000
      PRINT NNX, XM, NY, YM
      NEXT NY
      NEXT NNX
      RETURN

3000      IF WARN$ = "Y"
      THEN
!      PRINT #1 "WARNING: QMAX TOO HIGH"
      END IF
      CLOSE #1
3001      END

```

Figure 41. SPREAD.BAS: A program, written in VAX BASIC Version 3.3, used to read the data files created by SPACE.BAS.

```

100|*****
|*****
|
|
|          SPREAD.BAS
|          READS A POINT-TO-PLANE FILE
|
|*****
|*****
|*****
|          LIST OF VARIABLES
|*****
|*****
|
|          TIME:
|              T: Total time of calculation.
|              TSS: Selected time for snap-shot.
|              TSNAP:
|              TE:
|              TSTEP:
|              TTOT:
|
|          VOLTAGE:
|              VOLT: Integrated Potential
|
|          CURRENT:
|              CURRENT: Current per mm^2
|              CURR:
|              C: Total current
|
|          CHARGE:
|              Q:
|              QNUM:
|              QSUMNUM:
|              QGAPNUM:
|              QT:
|
|          POSITION:
|              XMIN:
|              XMAX:
|              D:
|              DP:
|
|          FIELD:
|              EX: Field strength (x-component).
|              EY: Field strength (y-component).
|
|          AREA:
|
|          COUNTERS:
|              NNX: Counter in x-direction.
|              NY: Counter in y-direction.
|              NCX: Number of x-grids.
|              NCY: Number of y-grids.
|
|          MISC:
|              ADIS:
|              RDEG:
|              PK$: Calculation type (PROF or SMALL)
|              FILE$: File to be read.
|              GRID$: Selected geometry (PARA or SQ).
|
|          CONSTANTS:

```

```

|
| ZKAPPA: Ion mobility
| *****
| *****
| *****
DIM X(15,15), Y(15,15), EX(15,15), EY(15,15), QT(15,15)
DIM T(100), VOLT(100), CURR(100), QS(100), QSG(100), Q(15)
DIM SURF(15), CURRENT(15)

200 INPUT "Name of file ", FILE$
INPUT "Cell print-out (Y/N) ", P2$
IF (P2$="y" or P2$="n") !ASSURE SHIFT LOCK
THEN
PRINT "Set 'Caps Lock'"
GOTO 200
END IF
INPUT "Current profile (Y/N) ", P3$
INPUT "What calculations? (PROF/SMALL) ", PK$
ZKAPPA=1.0E-4

!Open a file for input. Display introductory information.
GOSUB 2800 !SNAPINI
PRINT "2-D space charge calculation"
PRINT "File name ", FILE$
PRINT "Grid-type= ", GRID$
PRINT "D= ", D
PRINT "DP= ", DP
PRINT "NCX "; NCX, "NCY "; NCY
PRINT "ADIS ", ADIS
PRINT "TSNAP= "; TSNAP, "TE= "; TE
PRINT "TSTEP= "; TSTEP, "TTOT= "; TTOT

NS=0
IT=0
!NEWSN2:
400 INPUT "NEXT SNAP-SHOT?(Y/N)", TS$
IF TS$="Y"
THEN
GOTO 500
ELSE
GOTO 700
END IF

!NEWSN3:
500 NS=NS+1
!Trap errors.
ON ERROR GOTO 600
GOSUB 2900 !SNAP Read data from file.
IF T(NS) < (TSS-1E-5) THEN GOTO 500 END IF !NEWSN3
GOSUB 2400 !WCALC Direct the desired processing of information.
GOTO 400 !NEWSN2

600 IF ERR=11 THEN RESUME 650 !Deal with trapped EOF error.
ELSE RESUME 690 !Deal with other errors.
END IF
650 PRINT "END OF FILE (EOF) REACHED"
GOTO 700
690 PRINT "UNEXPECTED ERROR";ERR
700 CLOSE #1
GOTO 3100

| *****
| *****
| SUBROUTINE SECTION
| *****
| *****

```

Figure 41. SPREAD.BAS-continued

```

!
!   WCALC: Inquires about a choice of a desired calculation.
!           Accessed by GOSUB 2400
!
!   PROF: Creates a current profile on the counter-electrode.
!           Accessed by GOSUB 2500
!
!   PSMALL: Does a "small print-out" of the "snap" result.
!           Accessed by GOSUB 2600
!
!   SNAPINI: Reads the data-head from the SNAP-file.
!           Accessed by GOSUB 2800
!
!   SNAP: Inputs the electric field distribution from the SNAP file.
!           Accessed by GOSUB 2900
!
!   CALC: Performs current calculations based on field and charge data.
!           Accessed by GOSUB 3000
!
!*****
!*****
!*****
!   Subroutine WCALC: Inquires about choice of a desired calculation.
!   Accessed by GOSUB 2400
!*****
!*****

2400  !which calculation?
      IF PK$="PROF"           !Display current profile data.
      THEN
        GOSUB 2500 !PROF
      ELSE
        GOSUB 2600 !PSMALL    !Display "small output" of SNAP-file data.
      END IF
      RETURN

!*****
!   Subroutine PROF: Displays current profile on counter-electrode.
!   Accessed by GOSUB 2500
!*****
!*****

2500  NY=1
      PRINT T
      PRINT "Snap number ", NS
      PRINT "Time          ", T(NS)
      PRINT "NNX", "AREA", "AMPS", "AMPS/mm^2"
      FOR NNX=1 TO NCX
        IF NNX=1
          THEN
            XMIN=0
          ELSE
            XMIN=(NNX-1.5)*DP
          END IF
          XMAX=(NNX-0.5)*DP
          SURF(NNX)=3.1415*(XMAX*XMAX-XMIN*XMIN)
          C=-ZKAPPA*EY(NNX,NY)/(D/NCY)*QT(NNX,NY)
          CURRENT(NNX)=C/SURF(NNX)*1E-6    !current per mm2
          PRINT NNX, SURF(NNX), C, CURRENT(NNX)
        NEXT NNX
      RETURN

!*****
!   Subroutine PSMALL: Display a small print-out of the snap result.
!   Accessed by GOSUB 2600
!*****
!*****

```

Figure 41. SPREAD.BAS-continued

```

2600  PRINT
      PRINT "Snap number ", NS
      PRINT "Time      ", T(NS)
      PRINT "NNX", "NNY", "QT", "EX", "EY"
      FOR NY=0 TO NCY+1
        CURR=0
        IF P2$="Y"
          THEN
            FOR NNX=0 TO NCX+1
              !Q(NNX)=CSNG(QNUM(NNX,NY))
              !Q(NNX)=QNUM(NNX,NY)
              PRINT NNX, NY, QT(NNX, NY), EX(NNX,NY), EY(NNX,NY)
            NEXT NNX
          END IF
          FOR NNX=1 TO NCX
            CURR=CURR+EY(NNX,NY)*ZKAPPA*QT(NNX, NY)/(D/NCY)
          NEXT NNX
          IF P3$="Y"
            THEN
              PRINT "Current at NY= "; NY; " is "; CURR
            END IF
          IF P2$="Y" THEN INPUT "Pause ", P END IF
        NEXT NY

      GOSUB 3000 !CALC
      PRINT "V,center= "; VOLT(NS), "I,plate= "; CURR(NS)
      PRINT "Q-sum "; QS(NS); " Q-gap "; QSG(NS)
      RETURN

!*****
!      Subroutine SNAPINI: Reads the data-head from the SNAP-file.
!      Accessed by GOSUB 2800
!*****

2800  OPEN FILE$ FOR INPUT AS #1
      PRINT "SNAPINI subroutine"
      INPUT #1, GRID$
      INPUT #1, T1$          !"point-to-plane corona"
      IF GRID$="SQ"
        THEN
          PRINT "Square coordinate system"
          INPUT #1, D, DP, NCY, NCX, ADIS
        ELSE
          IF GRID$="PARA"
            THEN
              PRINT "Parabolic coordinate system"
              INPUT #1, D, DP, NCY, NCX, RDEG
            END IF
          END IF
          INPUT #1, TSNAP, TE, TSTEP, TTOT
          INPUT #1, ZJO
          FOR NNX=1 TO NCX
            INPUT #1, QD(NNX)
          NEXT NNX
!SNAP11:
      RETURN

!*****
!      Subroutine SNAP: Inputs the electric field distribution
!                      from the SNAP file.
!      Accessed by GOSUB 2900
!*****

2900  INPUT #1, T2$, T(NS)    !"T= "
      PRINT T2$, NS, T(NS)

```

Figure 41. SPREAD.BAS-continued

```

      INPUT #1, T3$           !"ELECTRIC FIELD AND CHARGE DISTRIBUTIONS"
      INPUT #1, T4$, QSUMNUM  !"Q,sum= "
      INPUT #1, T5$, QGAPNUM  !"Q,gap= "
      QS(NS)=QSUMNUM
      QSG(NS)=QGAPNUM
      PRINT "I", "J", "E_x", "QT"
      FOR NY=1 TO NCY
      FOR NNX=1 TO NCX
      INPUT #1, I, J, EX(NNX,NY), EY(NNX,NY), QT(NNX,NY)
      PRINT I, J, EX(NNX,NY), QT(NNX,NY)
      NEXT NNX
      NEXT NY
      NNX=0
      PRINT "I", "J", "QT"
      FOR NY=0 TO NCY+1
      INPUT #1, I, J, QT(NNX,NY)
      PRINT I, J, QT(NNX,NY)
      NEXT NY
      NNX=NCX+1
      FOR NY=0 TO NCY+1
      INPUT #1, NNX, NY, QT(NNX,NY)
      PRINT NNX, NY, QT(NNX,NY)
      NEXT NY
      NY=0
      FOR NNX=1 TO NCX
      INPUT #1, NNX, NY, QT(NNX,NY)
      PRINT NNX, NY, QT(NNX,NY)
      NEXT NNX
      NY=NCY+1
      FOR NNX=1 TO NCX
      INPUT #1, NNX, NY, QT(NNX,NY)
      PRINT NNX, NY, QT(NNX,NY)
      NEXT NNX
      RETURN

!*****
!      Subroutine CALC: Performs calculations of potential and current.
!      Accessed by GOSUB 3000
!*****

3000  NNX=1
      ESUM=0
      FOR NY=1 TO NCY
      ESUM=ESUM+EY(NNX,NY)
      NEXT NY
      VOLT(NS)=ESUM*D/NCY
      NY=1
      CURR(NS)=0
      FOR NNX=1 TO NCX
      CURR(NS)=CURR(NS)-EY(NNX,NY)*ZKAPPA*QT(NNX,NY)/(D/NCY)
      NEXT NNX
      RETURN

3100  !end program
      PRINT "THIS IS THE END"

      END

```

Figure 42. TUBE.M: A program, written for the command language of the MATLAB program, used to simulate ion flow through a drift tube.

```
%
% TUBE: A program to simulate the flow of ions, of one speciesm, through
% a drift tube.
%

%
% Input information about the drift tube and the ions produced in it.
% Also, initialize some of the variables, constants, etc.
%

N = input('no. of grid points= ');      %Tube is divided into N slices.
steps = input('no. of time steps= ');    %Number of time steps.
time(1)=0;                               %Initial time.
po = input('space charge= ');            %Space charge per "slice."
rho = diag(zeros(N));                    %Space charge vector.
l = input('length(meters)= ');           %Length of drift tube.
chg = input('plate charge= ');           %Difference between charges on plates.
thick = l/N;                             %Thickness of a slice.
a = input('distance from repeller to gate (meters)= ');
m = a/thick;                             %Number of slices on the source side
                                         %of the gate.

%
% Set up the initial conditions for the simulation.
%

for x=1:m
    rho(x) = po;                         %Fill the region with space charge.
end
vo = velocity(rho,m,N,chg);              %Call "velocity" to calculate the
                                         %velocity of ions in the fastest slice.
timestep = thick/vo;                     %Determin a timestep to give manageable
                                         %drift distance.

%
% Move the ions according to field condntions.
%

for time_inc=2:steps
    rho_new=diag(zeros(N+1));            %"New" space charge vector.
    if sum(rho) > po/1e10                %Condition for the end of the
                                         %simulation is the exit of most of the
                                         %space charge to the collector plate.
        for c=1:N
            if rho(c) ~= 0
                v(c) = velocity(rho,c,N,chg);
                %Calculate the average velocity of ion
                %drift in a "slice," c.
                rho_add = displacement(v(c),rho(c),thick,timeste
p,c,N);
                %Translate ion drift veloctiy into
                %distance of movement during a timestep.
                rho_new = rho_new + rho_add(1:N+1);
                %Report the ion displacement in terms
                %of a space charge vector.
            end
        end
    end

%
% Increment time.
%

time(time_inc) = time(time_inc-1)+timestep;
                                         %Accumulated time after the gate is
                                         %opened.
```

Figure 42. TUBE.M-continued

```

%
% Count the collected ions.
%
    collect(time_inc) = rho_new(N+1);
                                %Collected ions are ions that make it to
                                %the last cell of the drift tube.
    rho = rho_new(1:N);        %The new space charge vector, resulting
                                %from the summing of the displacements,
                                %is used for the next time step.
                                %end
end
clt = collect./timestep;      %Collector current:
                                % (number of ions collected/
                                % length of collection period.

%
% Plot the calculated data.
%
plot(time,clt)
title('Collector Current as a function of time after pulse')
ylabel('Current(ions/sec)')
xlabel('time(sec.)')

```

Figure 43. TUB2.M: A program, written for the command language of the MATLAB program, used to simulated the flow of a group of ions, having two different ion mobilities, through a drift tube.

```

%
% TUB2: A program to simulate the movement of two different kinds of ions, of
% differing mobilities, through a drift tube.
%

%
% Input information about the drift tube and the ions produced in it.
% Also, initialize some of the variables, constants, etc.
%

N = input('no. of grid points= '); %Tube is divided into N slices.
steps = input('no. of time steps= '); %Number of time steps.
time(1)=0; %Initial time.
poa = input('space charge of a= '); %Space charge per "slice."
pob = input('space charge of b= ');
rho = diag(zeros(N)); %Space charge vectors.
rhoa = diag(zeros(N));
rhob = diag(zeros(N));
ka = input('mobility of a= '); %Ion mobilities.
kb = input('mobility of b= ');
l = input('length(meters)= '); %Length of drift tube.
chg = input('plate charge= '); %Difference between charges on plates.
thick = l/N; %Thickness of a slice.
a = input('distance from repeller to gate(meters)= ');
m = a/thick; %Number of slices on the source side
%of the gate.

%
% Set up the initial conditions for the simulation.
%

for x=1:m
    rho(x) = poa+pob; %Fill the region with space charge.
    rhoa(x) = poa;
    rhob(x) = pob;
end
%vo = velocity(rho,m,N,chg); %Call "velocity" to calculate the
%velocity of ions in the fastest slice.
vov = vel_ion(rhoa,m,N,chg,ka);
vob = vel_ion(rhob,m,N,chg,kb);
if vov < vob
    timestep = thick/vob; %Determin a timestep to give manageable
%drift distance.
else
    timestep = thick/vov;
end

%
% Move the ions according to the field conditions.
%

for time_inc=2:steps
    rho_new = diag(zeros(N+1)); %"New" space charge vector.
    rhoa_new = diag(zeros(N+1));
    rhob_new = diag(zeros(N+1));
    if sum(rho) > poa/1e10 %Condition for the end of the
%simulation is the exit of most of the
%space charge to the collector plate.
        for c=1:N
            if rho(c) ~= 0
                vb(c) = vel_ion(rho,c,N,chg,kb);
                va(c) = vel_ion(rho,c,N,chg,ka);
                %Calculate the average velocity of ion
                %drift in a "slice," c.
                rhoa_add = displacement(va(c),rhoa(c),thick,time
step,c,N);
            end
        end
    end
    rho = rho_new;
    rhoa = rhoa_new;
    rhob = rhob_new;
end

```

Figure 43. TUB2.M-continued

```

step,c,N);

                                rhob_add = displacement(vb(c),rhob(c),thick,time
                                %Translate ion drift velocity into
                                %distance of movement during a timestep.
                                rhoa_new = rhoa_new + rhoa_add(1:N+1);
                                rhob_new = rhob_new + rhob_add(1:N+1);
                                %Report the ion displacement in terms
                                %of a space charge vector.
                                end
                                end
                                end

%
% Increment time.
%

time(time_inc) = time(time_inc-1)+timestep;
                                %Accumulated time after the gate is
                                %opened.

%
% Count the ions as they are collected.
%

collect(time_inc) = rhoa_new(N+1) + rhob_new(N+1);
                                %Collected ions are ions that make it to
                                %the last cell of the drift tube.
                                rhoa = rhoa_new(1:N);
                                rhob = rhob_new(1:N);
                                rho = rhoa + rhob;
                                %The new space charge vector, resulting
                                %from the summing of the displacements,
                                %is used for the next time step.
                                %end
end
clt = collect./timestep;
                                %Collector current:
                                %(number of ions collected/
                                % length of collection period.

%
% Plot the calculated data.
%

plot(time,clt)
title('Collector Current as a function of time after pulse')
ylabel('Current (ions/sec)')
xlabel('time(sec.)')

```

Figure 44. VELOCITY.M: A function, called by both TUBE.M and TUB2.M, used to calculate ion velocities.

[illegible]

Figure 45. DISPLACEMENT.M: A function, called by both TUBE.M and TUB2.M, used to calculate ion movements from cell to cell.

[illegible]

MONTANA STATE UNIVERSITY LIBRARIES



3 1762 10098521 5

HOUCHE
BINDERY L
UTICA/OMAH
NE.